

Contents

Bibliography	1
1 Formal Models and Tests	4
1.1 Formal Testing	4
1.2 Classical model for single measurements	5
1.3 Model for single measurement observations	6
1.4 Morgan Pitman	6
1.5 Identifiability	8
1.6 Measurement Error Models	8
1.7 Move to Chapter 3	9
1.8 Carstensen Model for Replicate Measurements	10
1.9 Paired sample t test	11
2 Regression Procedures	12
2.1 Regression Methods	12
2.1.1 Decomposition of Inter-Method Bias	13
2.1.2 Inference Procedures	13
2.2 Incorrect Techniques: Simple Linear Regression	14
2.2.1 Regression Analysis	14
2.2.2 The Identity Plot	14
2.2.3 Advantages of Regression Approaches for MCS	14
2.2.4 Disadvantages	15

2.3	Blackwood-Bradley Model	15
2.4	Bradley-Blackwood Method	17
2.4.1	Application to the Grubbs' Data	17
2.5	Bradley-Blackwood Test (Kevin Hayes Talk)	18
2.6	Error-In-Variable Models	18
2.7	Deming Regression	19
2.7.1	Kummel's Estimates	20
2.8	Deming Regression	22
2.9	Zhange Example	23
2.10	Model Evaluation for Deming Regression	23
2.11	Other Proposals for Formal Testing	25
2.12	Formal Models and Tests	27
2.13	Thompson 1963: Model Formulation and Formal Testing	27
2.14	Structural Equation Modelling	30
3	Error In Variable Models	32
3.1	Background	32
3.2	Model I and II Regression	32
3.2.1	Model I regression [Criterion v Test]	33
3.2.2	Model II regression [Test V Test]	34
3.2.3	Contention	35
3.3	Deming Regression	36
3.4	Error-In-Variable Models for Regression	36
3.4.1	Computational Aspects of Deming Regression	36
3.4.2	Variance Ratio	36
3.4.3	Estimating the Variance ratio	36
3.4.4	Inferences for Deming Regression	38
3.4.5	Expanding the use of Deming Regression for MCS	38
3.5	Performance in the presence of outliers	38

3.6	Using LME models to estimate the ratio (BXC)	39
3.7	Linnet - References	39
3.8	Ordinary Least Product Regression	40
3.9	Least Products Regression	40

Chapter 1

Formal Models and Tests

1.1 Formal Testing

The Bland-Altman plot is a simple tool for inspection of the data, but in itself offers little in the way of formal testing. It is upon the practitioner opinion to judge the outcome of the methodology.

The approach proposed by Altman and Bland (1983) is a formal test on the Pearson correlation coefficient of case-wise differences and means (ρ_{AD}). According to the authors, this test is equivalent to the ‘Pitman Morgan Test’.

For the Grubbs data, the correlation coefficient estimate (r_{AD}) is 0.2625, with a 95% confidence interval of (-0.366, 0.726) estimated by Fishers ‘r to z’ transformation (Cohen, Cohen, West, and Aiken, Cohen et al.). The null hypothesis ($\rho_{AD} = 0$) would fail to be rejected. Consequently the null hypothesis of equal variances of each method would also fail to be rejected. There has been no further mention of this particular test in Bland and Altman (1986), although Bland and Altman (1999) refers to Spearman’s rank correlation coefficient. Bland and Altman (1999) comments ‘we do not see a place for methods of analysis based on hypothesis testing’. Bland and Altman (1999) also states that consider structural equation models to be inappropriate.

1.2 Classical model for single measurements

Before continuing, we require a simple model to describe a measurement by method m . Carstensen (2004) presents a model to describe the relationship between a value of measurement and its real value. The non-replicate case is considered first, as it is the context of the Bland Altman plots. This model assumes that inter-method bias is the only difference between the two methods.

This model is based on measurements y_{mi} by method $m = 1, 2$ on item $i = 1, 2, \dots$. We use the term *item* to denote an individual, subject or sample, to be measured, being randomly sampled from a population

$$y_{mi} = \alpha_m + \mu_i + e_{mi}, \quad e_{mi} \sim \mathcal{N}(0, \sigma_m^2). \quad (1.1)$$

Here α_m is the fixed effect associated with method m , μ_i is the true value for subject i (fixed effect) and e_{mi} is a random effect term for errors.

The case-wise differences and means are calculated as $d_i = x_i - y_i$ and $a_i = (x_i + y_i)/2$ respectively. Both d_i and a_i are assumed to follow a bivariate normal distribution with $E(d_i) = \mu_d = \mu_1 - \mu_2$ and $E(a_i) = \mu_a = (\mu_1 + \mu_2)/2$. The variance matrix $\Sigma_{(a,d)}$ is

$$\Sigma_{(a,d)} = \begin{bmatrix} \sigma_1^2 + \sigma_2^2 & \frac{1}{2}(\sigma_1^2 - \sigma_2^2) \\ \frac{1}{2}(\sigma_1^2 - \sigma_2^2) & \sigma^2 + \frac{1}{4}(\sigma_1^2 + \sigma_2^2) \end{bmatrix}. \quad (1.2)$$

Likewise the separate α can not be estimated, only their difference can be estimated as \bar{d} (i.e. the inter-method bias). This model implies that the difference between the paired measurements can be expressed as

$$d_i = y_{1i} - y_{2i} \sim \mathcal{N}(\alpha_1 - \alpha_2, \sigma_1^2 + \sigma_2^2).$$

Importantly, this is independent of the item levels μ_i . As the case-wise differences are of interest, the parameters of interest are the fixed effects for methods α_m .

1.3 Model for single measurement observations

Kinsella (1986) formulates a model for single measurement observations for a method comparison study as a linear mixed effects model, i.e. model that additively combine fixed effects and random effects.

$$Y_{ij} = \mu + \beta_j + u_i + \epsilon_{ij} \quad i = 1, \dots, n \quad j = 1, 2$$

The true value of the measurement is represented by μ while the fixed effect due to method j is β_j . For simplicity these terms can be combined into single terms; $\mu_1 = \mu + \beta_1$ and $\mu_2 = \mu + \beta_2$. The inter-method bias is the difference of the two fixed effect terms, $\beta_1 - \beta_2$. Each individual is assumed to give rise to a random error, represented by u_i . This random effects term is assumed to have mean zero and be normally distributed with variance σ^2 . There is assumed to be an attendant error for each measurement on each individual, denoted ϵ_{ij} . This is also assumed to have mean zero. The variance of measurement error for both methods are not assumed to be identical for both methods variance, hence it is denoted σ_j^2 . The set of observations (x_i, y_i) by methods X and Y are assumed to follow a bivariate normal distribution with expected values $E(x_i) = \mu_i$ and $E(y_i) = \tau_i$ respectively. The variance covariance of the observations Σ is given by

$$\Sigma = \begin{bmatrix} \sigma^2 + \sigma_1^2 & \sigma^2 \\ \sigma^2 & \sigma^2 + \sigma_2^2 \end{bmatrix}$$

1.4 Morgan Pitman

An early contribution to formal testing in method comparison was made by both Morgan (1939) and Pitman (1939), in separate contributions. This test assess the equality of population variances. Pitman's test tests for zero correlation between the sums and products. The basis of this approach is that the distribution of the original measurements is bivariate normal. Correlation between differences and means is a test statistics for the null hypothesis of equal variances given bivariate normality.

The test of the hypothesis that the variances σ_1^2 and σ_2^2 are equal, which was devised concurrently by Pitman (1939) and Morgan (1939), is based on the correlation of the casewise-differences and sums, d with s , the coefficient being $\rho_{(d,s)} = (\sigma_1^2 - \sigma_2^2)/(\sigma_D \sigma_S)$, which is zero if, and only if, $\sigma_1^2 = \sigma_2^2$. The classical Pitman-Morgan test can be adapted for the correlation value $\rho_{(a,d)}$, and is evaluated as follows;

$$\rho(a, d) = \frac{\sigma_1^2 - \sigma_2^2}{\sqrt{(\sigma_1^2 + \sigma_2^2)(4\sigma_S^2 + \sigma_1^2 + \sigma_2^2)}} \quad (1.3)$$

The basis of this approach is that the distribution of the original measurements is bivariate normal. Morgan and Pitman noted that the correlation coefficient depends upon the difference $\sigma_1^2 - \sigma_2^2$, being zero if and only if $\sigma_1^2 = \sigma_2^2$.

The test of the hypothesis that the variance of both methods are equal is based on the correlation value $\rho_{D,A}$ which is evaluated as follows;

$$\rho(D, A) = \frac{\sigma_1^2 - \sigma_2^2}{\sqrt{(\sigma_1^2 + \sigma_2^2)(4\sigma_S^2 + \sigma_1^2 + \sigma_2^2)}} \quad (1.4)$$

The correlation constant takes the value zero if, and only if, the two variances are equal. Therefore a test of the hypothesis $H : \sigma_1^2 = \sigma_2^2$ is equivalent to a test of the hypothesis $H : \rho(D, A) = 0$. This corresponds to the well-known t test for a correlation coefficient with $n - 2$ degrees of freedom.

The classical Pitman-Morgan test is a hypothesis test for equality of the variance of two data sets; $\sigma_1^2 = \sigma_2^2$, based on the correlation value $\rho_{a,d}$, and is evaluated as follows;

$$\rho(a, d) = \frac{\sigma_1^2 - \sigma_2^2}{\sqrt{(\sigma_1^2 + \sigma_2^2)(4\sigma_S^2 + \sigma_1^2 + \sigma_2^2)}} \quad (1.5)$$

The correlation constant takes the value zero if, and only if, the two variances are equal.

Morgan and Pitman noted that the correlation coefficient depends upon the difference $\sigma_1^2 - \sigma_2^2$, being zero if and only if $\sigma_1^2 = \sigma_2^2$. Therefore a test of the hypothesis $H : \sigma_1^2 = \sigma_2^2$ is equivalent to a test of the hypothesis $H : \rho(D, A) = 0$. This corresponds to the well-known t test for a correlation coefficient with $n - 2$ degrees of freedom.

Bartko (1994) describes the Morgan-Pitman test as identical to the test of the slope equal to zero in the regression of Y_{i1} on Y_{i2} , a result that can be derived using straightforward algebra. The Pitman-Morgan test is equivalent to the marginal test of the slope estimate in Bradley-Blackwoods model.

The Pitman-Morgan test for equal variances is based on the correlation of D with S. The correlation coefficient is zero if, and only if, the variances are equal. The test statistic is the familiar t-test with $n-2$ degree of freedom.

Bradley and Blackwood (1989) construct the conditional expectation of D given S as linear model. They used this result to propose a test of the joint hypothesis of the mean difference and equal variances. If the intercept and slope estimates are zero, the two methods have the same mean and variance.

1.5 Identifiability

Dunn (2002) highlights an important issue regarding using models such as structural equation modelling, which is the identifiability problem. This comes as a result of there being too many parameters to be estimated. Therefore assumptions about some parameters, or estimators used, must be made so that others can be estimated. For example, in the literature, the variance ratio $\lambda = \frac{\sigma_1^2}{\sigma_2^2}$ must often be assumed to be equal to 1 (Linnet, 1998). Dunn (2002) considers approaches based on two methods with single measurements on each subject as inadequate for a serious study on the measurement characteristics of the methods. This is because there would not be enough data to allow for a meaningful analysis. There is, however, a counter-argument that in many practical settings it is very difficult to get replicate observations when, for example, the measurement method requires invasive medical procedure.

1.6 Measurement Error Models

Dunn (2002) proposes a measurement error model for use in method comparison stud-

ies. Consider n pairs of measurements X_i and Y_i for $i = 1, 2, \dots, n$.

$$X_i = \tau_i + \delta_i \quad (1.6)$$

$$Y_i = \alpha + \beta\tau_i + \epsilon_i$$

In the above formulation is in the form of a linear structural relationship, with τ_i and $\beta\tau_i$ as the true values, and δ_i and ϵ_i as the corresponding measurement errors. In the case where the units of measurement are the same, then $\beta = 1$.

$$E(X_i) = \tau_i \quad (1.7)$$

$$E(Y_i) = \alpha + \beta\tau_i$$

$$E(\delta_i) = E(\epsilon_i) = 0$$

The value α is the inter-method bias between the two methods.

$$z_0 = d = 0 \quad (1.8)$$

$$z_{n+1} = z_n^2 + c \quad (1.9)$$

1.7 Move to Chapter 3

Carstensen (2004) also advocates the use of linear mixed models in the study of method comparisons. The model is constructed to describe the relationship between a value of measurement and its real value. The non-replicate case is considered first, as it is the context of the Bland-Altman plots. This model assumes that inter-method bias is the only difference between the two methods. A measurement y_{mi} by method m on individual i is formulated as follows;

$$y_{mi} = \alpha_m + \mu_i + e_{mi} \quad (e_{mi} \sim N(0, \sigma_m^2)) \quad (1.10)$$

The differences are expressed as $d_i = y_{1i} - y_{2i}$. For the replicate case, an interaction term c is added to the model, with an associated variance component. All the random

effects are assumed independent, and that all replicate measurements are assumed to be exchangeable within each method.

$$y_{mir} = \alpha_m + \mu_i + c_{mi} + e_{mir} \quad (e_{mi} \sim N(0, \sigma_m^2), c_{mi} \sim N(0, \tau_m^2)) \quad (1.11)$$

1.8 Carstensen Model for Replicate Measurements

Carstensen et al. (2008) develop their model from a standard two-way analysis of variance model, reformulated for the case of replicate measurements, with random effects terms specified as appropriate. For the replicate case, an interaction term c is added to the model, with an associated variance component. Their model describing y_{mir} , again the r th replicate measurement on the i th item by the m th method ($m = 1, 2$, $i = 1, \dots, N$, and $r = 1, \dots, n$), can be written as

$$y_{mir} = \alpha_m + \mu_i + a_{ir} + c_{mi} + \epsilon_{mir}. \quad (1.12)$$

Again, the fixed effects α_m and μ_i represent the intercept for method m and the ‘true value’ for item i respectively. The random-effect terms comprise an item-by-replicate interaction term $a_{ir} \sim \mathcal{N}(0, \varsigma^2)$, a method-by-item interaction term $c_{mi} \sim \mathcal{N}(0, \tau_m^2)$, and model error terms $\epsilon \sim \mathcal{N}(0, \varphi_m^2)$. All random-effect terms are assumed to be independent. For the case when replicate measurements are assumed to be exchangeable for item i , a_{ir} can be removed.

The model expressed in (2) describes measurements by m methods, where $m = \{1, 2, 3 \dots\}$. Based on the model expressed in (2), Carstensen et al. (2008) compute the limits of agreement as

$$\alpha_1 - \alpha_2 \pm 2\sqrt{\tau_1^2 + \tau_2^2 + \varphi_1^2 + \varphi_2^2}$$

Carstensen et al. (2008) notes that, for $m = 2$, separate estimates of τ_m^2 can not be obtained. To overcome this, the assumption of equality, i.e. $\tau_1^2 = \tau_2^2$ is required.

$$y_{mir} = \alpha_m + \mu_i + c_{mi} + e_{mir}, \quad e_{mi} \sim \mathcal{N}(0, \sigma_m^2), \quad c_{mi} \sim \mathcal{N}(0, \tau_m^2). \quad (1.13)$$

1.9 Paired sample t test

Bartko (1994) discusses the use of the well known paired sample t test to test for inter-method bias; $H : \mu_d = 0$. The test statistic is distributed a t random variable with $n - 1$ degrees of freedom and is calculated as follows,

$$t^* = \frac{\bar{d}}{\frac{s_d}{\sqrt{n}}} \quad (1.14)$$

where \bar{d} and s_d is the average of the differences of the n observations. Only if the two methods show comparable precision then the paired sample student t -test is appropriate for assessing the magnitude of the bias.

Chapter 2

Regression Procedures

2.1 Regression Methods

Conventional regression models are estimated using the ordinary least squares (OLS) technique, and are referred to as ‘Model I regression’ (Cornbleet and Cochrane, 1979; Ludbrook, 1997). A key feature of Model I models is that the independent variable is assumed to be measured without error. As often pointed out in several papers (Altman and Bland, 1983; Ludbrook, 1997), this assumption invalidates simple linear regression for use in method comparison studies, as both methods must be assumed to be measured with error.

The use of regression models that assumes the presence of error in both variables X and Y have been proposed for use instead (Cornbleet and Cochrane, 1979; Ludbrook, 1997). These methodologies are collectively known as ‘Model II regression’. They differ in the method used to estimate the parameters of the regression.

Regression estimates depend on formulation of the model. A formulation with one method considered as the X variable will yield different estimates for a formulation where it is the Y variable. With Model I regression, the models fitted in both cases will entirely different and inconsistent. However with Model II regression, they will be consistent and complementary.

Regression approaches are useful for a making a detailed examination of the biases across the range of measurements, allowing bias to be decomposed into fixed bias and proportional bias. Fixed bias describes the case where one method gives values that are consistently different to the other across the whole range. Proportional bias describes the difference in measurements getting progressively greater, or smaller, across the range of measurements. A measurement method may have either an attendant fixed bias or proportional bias, or both. (?). Determination of these biases shall be discussed in due course.

2.1.1 Decomposition of Inter-Method Bias

Regression approaches are useful for a making a detailed examination of the biases across the range of measurements, allowing inter-method bias to be decomposed into fixed bias and proportional bias. Fixed bias describes the case where one method gives values that are consistently different to the other across the whole range.

Constant or proportional bias in method comparison studies using linear regression can be detected by an individual test on the intercept or the slope of the line regressed from the results of the two methods to be compared.

Proportional bias describes the difference in measurements getting progressively greater, or smaller, across the range of measurements. A measurement method may have either an attendant fixed bias or proportional bias, or both (Ludbrook, 2002).

If the basic assumptions underlying linear regression are not met, the regression equation, and consequently the estimations of bias are undermined. Outliers are a source of error in regression estimates.

2.1.2 Inference Procedures

A 95% confidence interval for the intercept estimate can be used to test the intercept, and hence fixed bias, is equal to zero. This hypothesis is accepted if the confidence interval for the estimate contains the value 0 in its range. Should this be, it can be

concluded that fixed bias is not present. Conversely, if the hypothesis is rejected, then it is concluded that the intercept is non zero, and that fixed bias is present.

Testing for proportional bias is a very similar procedure. The 95% confidence interval for the slope estimate can be used to test the hypothesis that the slope is equal to 1. This hypothesis is accepted if the confidence interval for the estimate contains the value 1 in its range. If the hypothesis is rejected, then it is concluded that the slope is significant different from 1 and that a proportional bias exists.

2.2 Incorrect Techniques: Simple Linear Regression

2.2.1 Regression Analysis

Another inappropriate approach is the regressing one set of measurements against the other. According to this methodology the measurement methods could considered equivalent if the confidence interval for the regression coefficient included 1. Analysts sometimes use least squares (referred to by Ludbrook as Model I) regression analysis to calibrate one method of measurement against another. In this technique, the sum of the squares of the vertical deviations of y values from the line is minimized. This approach is invalid, because both y and x values are attended by random error.

2.2.2 The Identity Plot

This is a simple graphical approach, advocated by Bland and Altman (1986), that yields a cursory examination of how well the measurement methods agree. In the case of good agreement, the co-variates of the plot accord closely with the $X = Y$ line.

2.2.3 Advantages of Regression Approaches for MCS

- These methods can be employed in conversion problems.

- Bland and Altman have stated that regression analysis offers insights into MCS problems.

2.2.4 Disadvantages

- Regression methods are uninformative about the variability of the differences.
- Regression methods can determine the presence of bias, and the levels of constant bias and proportional bias thereof Ludbrook (1997, 2002).
- **Constant Bias** This is a form of systematic deviations estimated as the average difference between the test and the reference method.
- **Proportional Bias** Two methods may agree on average, but they may exhibit differences over a range of measurements.

Two methods may agree on average, but they may exhibit differences over a range of measurements. Proportional Bias is a difference in the two measures which is proportional to the scale of the measurement.

Using a naive estimation of bias, such as the mean of differences, it may incorrectly indicate absence of bias, by yielding a mean difference close to zero. This would be caused by positive differences in the measurements at one end of the range of measurements being canceled out by negative differences at the other end of the scale.

2.3 Blackwood-Bradley Model

Bradley and Blackwood (1989) offers a formal simultaneous hypothesis test for the mean and variance of two paired data sets. Using simple linear regression of the differences of each pair against the sums, a line is fitted to the model, with estimates for intercept and slope ($\hat{\beta}_0$ and $\hat{\beta}_1$). The null hypothesis of this test is that the mean (μ) and variance (σ^2) of both data sets are equal if the slope and intercept estimates are equal to zero (i.e $\sigma_1^2 = \sigma_2^2$ and $\mu_1 = \mu_2$ if and only if $\beta_0 = \beta_1 = 0$)

Bradley and Blackwood (1989) have developed a regression based procedure for assessing the agreement. This approach performs a simultaneous test for the equivalence of means and variances of the respective methods. The Bradley Blackwood test is a simultaneous test for bias and precision. They propose a regression approach which fits D on M , where D is the difference and average of a pair of results. Using simple linear regression of the differences of each pair against the sums, a line is fitted to the model, with estimates for intercept and slope ($\hat{\beta}_0$ and $\hat{\beta}_1$).

$$D = (X_1 - X_2) \quad (2.1)$$

$$M = (X_1 + X_2)/2 \quad (2.2)$$

The Bradley Blackwood Procedure fits D on M as follows:

$$D = \beta_0 + \beta_1 M \quad (2.3)$$

This technique offers a formal simultaneous hypothesis test for the mean and variance of two paired data sets. The null hypothesis of this test is that the mean (μ) and variance (σ^2) of both data sets are equal if the slope and intercept estimates are equal to zero (i.e. $\sigma_1^2 = \sigma_2^2$ and $\mu_1 = \mu_2$ if and only if $\beta_0 = \beta_1 = 0$)

Both beta values, the intercept and slope, are derived from the respective means and standard deviations of their respective data sets.

We determine if the respective means and variances are equal if both beta values are simultaneously equal to zero. The Test is conducted using an F test, calculated from the results of a regression of D on M .

Russell et al have suggested this method be used in conjunction with a paired t-test , with estimates of slope and intercept.

Bradley and Blackwood have developed a regression based approach assessing the agreement.

We have identified this approach to be examined to see if it can be used as a foundation for a test perform a test on means and variances individually.

2.4 Bradley-Blackwood Method

A test statistic is then calculated from the regression analysis of variance values (Bradley and Blackwood, 1989) and is distributed as ‘ F ’ random variable. The degrees of freedom are $\nu_1 = 2$ and $\nu_2 = n - 2$ (where n is the number of pairs). The critical value is chosen for $\alpha\%$ significance with those same degrees of freedom. Bartko (1994) amends this methodology for use in method comparison studies, using the averages of the pairs, as opposed to the sums, and their differences. This approach can facilitate simultaneous usage of test with the Bland-Altman methodology. Bartko’s test statistic take the form:

$$F.test = \frac{(\Sigma d^2) - SSReg}{2MSReg}$$

2.4.1 Application to the Grubbs’ Data

For the Grubbs data, $\Sigma d^2 = 5.09$, $SSReg = 0.60$ and $MSreg = 0.06$ Therefore the test statistic is 37.42, with a critical value of 4.10. Hence the means and variance of the Fotobalk and Counter chronometers are assumed to be simultaneously equal.

Importantly, this approach determines whether there is both inter-method bias and precision present, or alternatively if there is neither present. It has previously been demonstrated that there is a inter-method bias present, but as this procedure does not allow for separate testing, no conclusion can be drawn on the comparative precision of both methods.

	Df	Sum Sq	Mean Sq	F value	Pr(>F)
Averages	1	0.04	0.04	0.74	0.4097
Residuals	10	0.60	0.06		

Table 2.4.1: Regression ANOVA of case-wise differences and averages for Grubbs Data

2.5 Bradley-Blackwood Test (Kevin Hayes Talk)

This work considers the problem of testing $\mu_1 = \mu_2$ and $\sigma_1^2 = \sigma_2^2$ using a random sample from a bivariate normal distribution with parameters $(\mu_1, \mu_2, \sigma_1^2, \sigma_2^2, \rho)$.

The new contribution is a decomposition of the Bradley-Blackwood test statistic (*Bradley and Blackwood, 1989*) for the simultaneous test of $\mu_1 = \mu_2$; $\sigma_1^2 = \sigma_2^2$ as a sum of two statistics.

One is equivalent to the Pitman-Morgan (*Pitman, 1939; Morgan, 1939*) test statistic for $\sigma_1^2 = \sigma_2^2$ and the other one is a new alternative to the standard paired-t test of $\mu_D = \mu_1 = \mu_2 = 0$.

Surprisingly, the classic Student paired-t test makes no assumptions about the equality (or otherwise) of the variance parameters.

The power functions for these tests are quite easy to derive, and show that when $\sigma_1^2 = \sigma_2^2$, the paired t-test has a slight advantage over the new alternative in terms of power, but when $\sigma_1^2 \neq \sigma_2^2$, the new test has substantially higher power than the paired-t test.

While Bradley and Blackwood provide a test on the joint hypothesis of equal means and equal variances their regression based approach does not separate these two issues.

The rejection of the joint hypothesis may be due to two groups with unequal means and unequal variances; unequal means and equal variances, or equal means and unequal variances. We propose an approach for resolving this (model selection) problem in a manner controlling the magnitudes of the relevant type I error probabilities.

2.6 Error-In-Variable Models

Conventional regression models are estimated using the ordinary least squares (OLS) technique, and are referred to as ‘Model I regression’ (Cornbleet and Cochrane, 1979; Ludbrook, 1997). A key feature of Model I models is that the independent variable is assumed to be measured without error. As often pointed out in several papers

(Altman and Bland, 1983; Ludbrook, 1997), this assumption invalidates simple linear regression for use in method comparison studies, as both methods must be assumed to be measured with error.

The use of regression models that assumes the presence of error in both variables X and Y have been proposed for use instead (Cornbleet and Cochrane, 1979; Ludbrook, 1997). These methodologies are collectively known as “Error-In-Variables Models” and “Model II regression”. They differ in the method used to estimate the parameters of the regression.

Errors-in-variables models or measurement errors models are regression models that account for measurement errors in the independent variables, as well as the dependent variable.

Regression estimates depend on formulation of the model. A formulation with one method considered as the X variable will yield different estimates for a formulation where it is the Y variable. With Model I regression, the models fitted in both cases will entirely different and inconsistent. However with Model II regression, they will be consistent and complementary.

Cornbleet and Cochrane (1979) comparing the three methods, citing studies by other authors, concluding that Deming regression is the most useful of these methods. They found the Bartlett method to be flawed in determining slopes.

However the author point out that *clinical laboratory measurements usually increase in absolute imprecision when larger values are measured*. However one of the assumptions that underline Deming and Mandel regression is constancy of the measurement errors throughout the range of values.

2.7 Deming Regression

As stated previously, the fundamental flaw of simple linear regression is that it allows for measurement error in one variable only. This causes a downward biased slope estimate.

Deming regression is a regression fitting approach that assumes error in both variables. Deming regression is recommended by Cornbleet and Cochrane (1979) as the preferred Model II regression for use in method comparison studies. The sum of squared distances from measured sets of values to the regression line is minimized at an angle specified by the ratio λ of the residual variance of both variables. When λ is one, the angle is 45 degrees. In ordinary linear regression, the distances are minimized in the vertical directions (Linnet, 1999). In cases involving only single measurements by each method, λ may be unknown and is therefore assumed a value of one. While this will produce biased estimates, they are less biased than ordinary linear regression.

The Bland Altman Plot is uninformative about the comparative influence of proportional bias and fixed bias. Model II approaches, such as Deming regression, can provide independent tests for both types of bias.

As with conventional regression methodologies, Deming regression calculates an estimate for both the slope and intercept for the fitted line, and standard errors thereof. Therefore there is sufficient information to carry out hypothesis tests on both estimates, that are informative about presence of fixed and proportional bias.

Deming regression method also calculates a line of best fit for two sets of data. It differs from simple linear regression in that it is derived in a way that factors in for error in the x-axis, as well as the y-axis. The sum of the square of the residuals of both variables are simultaneously minimized. This derivation results in the best fit to minimize the sum of the squares of the perpendicular distances from the data points. Normally distributed error of both variables is assumed, as well as a constant level of imprecision throughout the range of measurements.

2.7.1 Kummel's Estimates

For a given λ , Kummel (1879) derived the following estimate that would later be used for the Deming regression slope parameter. The intercept estimate α is simply estimated in the same way as in conventional linear regression, by using the identity

$$\bar{Y} - \hat{\beta}\bar{X};$$

$$\hat{\beta} = \frac{S_{yy} - \lambda S_{xx} + [(S_{yy} - \lambda S_{xx})^2 + 4\lambda S_{xy}^2]^{1/2}}{2S_{xy}} \quad (2.4)$$

, with λ as the variance ratio. As stated previously λ is often unknown, and therefore must be assumed to equal one.

The sum of squared distances from measured sets of values to the regression line is minimized at an angles specified by the ratio λ of the residual variance of both variables. The measurement error is specified with measurement error variance related as

$$\lambda = \sigma_y^2 / \sigma_x^2$$

where σ_x^2 and σ_y^2 is the measurement error variance of the x and y variables, respectively. The variance of the ratio, λ , specifies the angle. When λ is one, the angle is 45 degrees. This approach would be appropriate when errors in y and x are both caused by measurements, and the accuracy of measuring devices or procedures are known. In cases involving only single measurements by each method, λ may be unknown and is therefore assumes a value of one. While this will bias the estimates, it is less biased than ordinary linear regression.

Deming regression assumes that the ratio $\lambda = \sigma_\epsilon^2 / \sigma_\eta^2$ is known. In the case where λ is equal to one, (i.e. equal error variances), the methodology is equivalent to ***orthogonal regression***.

Carroll and Ruppert (1996) states that Deming regression is acceptable only when the precision ratio (λ , in their paper as η) is correctly specified, but in practice this is often not the case, with the λ being underestimated. Several candidate models, with varying variance ratios may be fitted, and estimates of the slope and intercept are produced. However no model selection information is available to determine the best fitting model.

As with conventional regression methodologies, Deming regression calculates an estimate for both the slope and intercept for the fitted line, and standard errors thereof. Therefore there is sufficient information to carry out hypothesis tests on both estimates,

that are informative about presence of fixed and proportional bias.

A 95% confidence interval for the intercept estimate can be used to test the intercept, and hence fixed bias, is equal to zero. This hypothesis is accepted if the confidence interval for the estimate contains the value 0 in its range. Should this be, it can be concluded that fixed bias is not present. Conversely, if the hypothesis is rejected, then it is concluded that the intercept is non zero, and that fixed bias is present.

Testing for proportional bias is a very similar procedure. The 95% confidence interval for the slope estimate can be used to test the hypothesis that the slope is equal to 1. This hypothesis is accepted if the confidence interval for the estimate contains the value 1 in its range. If the hypothesis is rejected, then it is concluded that the slope is significant different from 1 and that a proportional bias exists.

Carroll and Ruppert (1996) states that Deming's regression is acceptable only when the precision ratio (λ , in their paper as η) is correctly specified, but in practice this is often not the case, with the λ being underestimated.

2.8 Deming Regression

The most commonly known Model II methodology is known as Deming's Regression, (also known as Ordinary Least Product regression). Deming regression is recommended by Cornbleet and Cochrane (1979) as the preferred Model II regression for use in method comparison studies.

Informative analysis for the purposes of method comparison, Deming Regression is a regression technique taking into account uncertainty in both the independent and dependent variables. Deming's method always results in one regression fit, regardless of which variable takes the place of the predictor variables.

As with conventional regression methodologies, Deming regression calculates an estimate for both the slope and intercept for the fitted line, and standard errors thereof. Therefore there is sufficient information to carry out hypothesis tests on both estimates, that are informative about presence of fixed and proportional bias.

2.9 Zhange Example

For convenience, a new data set shall be introduced to demonstrate Deming regression. Measurements of transmitral volumetric flow (MF) by doppler echocardiography, and left ventricular stroke volume (SV) by cross sectional echocardiography in 21 patients with aortic valve disease are tabulated in Zhang et al. (1986). This data set features in the discussion of method comparison studies in Altman (1991, p.398) .

Patient	MF (cm^3)	SV (cm^3)	Patient	MF (cm^3)	SV (cm^3)	Patient	MF (cm^3)	SV (cm^3)
1	47	43	8	75	72	15	90	82
2	66	70	9	79	92	16	100	100
3	68	72	10	81	76	17	104	94
4	69	81	11	85	85	18	105	98
5	70	60	12	87	82	19	112	108
6	70	67	13	87	90	20	120	131
7	73	72	14	87	96	21	132	131

Table 2.9.2: Transmitral volumetric flow(MF) and left ventricular stroke volume (SV) in 21 patients. (Zhang et al 1986)

2.10 Model Evaluation for Deming Regression

Bootstrap techniques can be used to obtain Confidence Intervals for Deming regression estimates. Authors such as Carpenter and Bithell (2000) and Johnson (2001) provide relevant insights.

Model selection and diagnostic technique are well developed for classical linear regression methods. Typically an implementation of a linear model fit will be accompanied by additional information, such as the coefficient of determination and likelihood

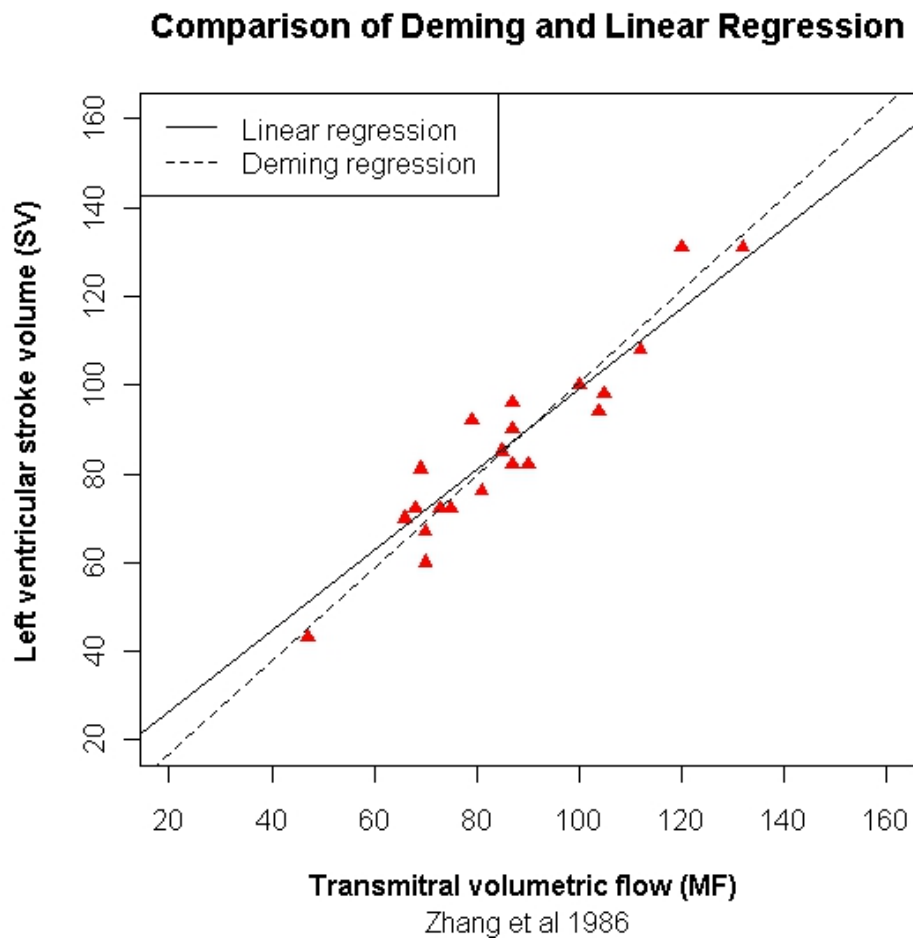


Figure 2.9.1: Deming Regression For Zhang's Data

and information criteria, and a regression ANOVA table. Such additional information has not, as yet, been implemented for Deming regression.

Deming's Regression suffers from some crucial drawbacks. Firstly it is computationally complex, and it requires specific software packages to perform calculations. Secondly, in common with all regression methods, Deming regression is vulnerable to outliers. Lastly, Deming regression is uninformative about the comparative precision of two methods of measurement. Most importantly Carroll and Ruppert (1996) states that Deming's regression is acceptable only when the precision ratio (λ , in their paper as η) is correctly specified, but in practice this is often not the case, with the λ being

underestimated. This underestimation leads to an overcorrection for attenuation.

2.11 Other Proposals for Formal Testing

Kinsella (1986) notes the lack of formal testing offered by this Bland-Altman plot. Furthermore, Kinsella (1986) formulates a model for single measurement observations as a linear mixed effects model, i.e. a model that additively combines fixed effects and random effects:

$$Y_{ij} = \mu + \beta_j + u_i + \epsilon_{ij} \quad i = 1, \dots, n \quad j = 1, 2$$

The true value of the measurement is represented by μ while the fixed effect due to method j is β_j . For simplicity these terms can be combined into single terms; $\mu_1 = \mu + \beta_1$ and $\mu_2 = \mu + \beta_2$. The inter-method bias is the difference of the two fixed effect terms, $\beta_1 - \beta_2$. Each individual is assumed to give rise to a random error, represented by u_i . This random effects term is assumed to have mean zero and be normally distributed with variance σ^2 . There is assumed to be an attendant error for each measurement on each individual, denoted ϵ_{ij} . This is also assumed to have mean zero. The variance of measurement error for both methods are not assumed to be identical for both methods variance, hence it is denoted σ_j^2 . The set of observations (x_i, y_i) by methods X and Y are assumed to follow a bivariate normal distribution with expected values $E(x_i) = \mu_i$ and $E(y_i) = \tau_i$ respectively. The variance covariance of the observations Σ is given by

$$\Sigma = \begin{bmatrix} \sigma^2 + \sigma_1^2 & \sigma^2 \\ \sigma^2 & \sigma^2 + \sigma_2^2 \end{bmatrix}$$

Kinsella (1986) demonstrates the estimation of the variance terms and relative precisions relevant to a method comparison study, with attendant confidence intervals for both. The measurement model introduced by Grubbs (1948, 1973) provides a formal procedure for estimating the variances σ^2 , σ_1^2 and σ_2^2 . Grubbs (1948) offers estimates,

commonly known as Grubbs estimators, for the various variance components. These estimates are maximum likelihood estimates, which shall be revisited in due course.

$$\begin{aligned}\hat{\sigma}^2 &= \sum \frac{(x_i - \bar{x})(y_i - \bar{y})}{n-1} = S_{xy} \\ \hat{\sigma}_1^2 &= \sum \frac{(x_i - \bar{x})^2}{n-1} = S^2_x - S_{xy} \\ \hat{\sigma}_2^2 &= \sum \frac{(y_i - \bar{y})^2}{n-1} = S^2_y - S_{xy}\end{aligned}$$

Thompson (1963) defines $\Delta_j = \sigma^2/\sigma_j^2, j = 1, 2$, to be a measure of the relative precision of the measurement methods, and demonstrates how to make statistical inferences about Δ_j . Based on the following identities,

$$\begin{aligned}C_x &= (n-1)S_x^2, \\ C_{xy} &= (n-1)S_{xy}, \\ C_y &= (n-1)S_y^2, \\ |A| &= C_x \times C_y - (C_{xy})^2,\end{aligned}$$

the confidence interval limits of Δ_1 are

$$\frac{C_{xy} - t(\frac{|A|}{n-2})^{\frac{1}{2}}}{C_x - C_{xy} + t(\frac{|A|}{n-2})^{\frac{1}{2}}} < \Delta_1 < \frac{C_{xy} + t(\frac{|A|}{n-2})^{\frac{1}{2}}}{C_x - C_{xy} - t(\frac{|A|}{n-1})^{\frac{1}{2}}}$$

The value t is the $100(1 - \alpha/2)\%$ upper quantile of Student's t distribution with $n - 2$ degrees of freedom (Kinsella, 1986). The confidence limits for Δ_2 are found by substituting C_y for C_x in (1.2). Negative lower limits are replaced by the value 0.

The case-wise differences and means are calculated as $d_i = x_i - y_i$ and $a_i = (x_i + y_i)/2$ respectively. Both d_i and a_i are assumed to follow a bivariate normal distribution with $E(d_i) = \mu_d = \mu_1 - \mu_2$ and $E(a_i) = \mu_a = (\mu_1 + \mu_2)/2$, and the variance matrix $\Sigma_{(a,d)}$ is

$$\Sigma_{(a,d)} = \begin{bmatrix} \sigma_1^2 + \sigma_2^2 & \frac{1}{2}(\sigma_1^2 - \sigma_2^2) \\ \frac{1}{2}(\sigma_1^2 - \sigma_2^2) & \sigma^2 + \frac{1}{4}(\sigma_1^2 + \sigma_2^2) \end{bmatrix}. \quad (2.5)$$

2.12 Formal Models and Tests

Thompson (1963) defines $\Delta_j = \sigma^2/\sigma_j^2, j = 1, 2$, to be a measure of the relative precision of the measurement methods, and demonstrates how to make statistical inferences about Δ_j . Based on the following identities,

$$\begin{aligned} C_x &= (n-1)S_x^2, \\ C_{xy} &= (n-1)S_{xy}, \\ C_y &= (n-1)S_y^2, \\ |A| &= C_x \times C_y - (C_{xy})^2, \end{aligned}$$

the confidence interval limits of Δ_1 are

$$\frac{C_{xy} - t(\frac{|A|}{n-2})^{\frac{1}{2}}}{C_x - C_{xy} + t(\frac{|A|}{n-2})^{\frac{1}{2}}} < \Delta_1 < \frac{C_{xy} + t(\frac{|A|}{n-2})^{\frac{1}{2}}}{C_x - C_{xy} - t(\frac{|A|}{n-2})^{\frac{1}{2}}}$$

The value t is the $100(1 - \alpha/2)\%$ upper quantile of Student's t distribution with $n - 2$ degrees of freedom (Kinsella, 1986). The confidence limits for Δ_2 are found by substituting C_y for C_x in (1.2). Negative lower limits are replaced by the value 0. The ratio Δ_2 can be found by interchanging C_y and C_x . A lower confidence limit can be found by calculating the square root. The inequality in equation 1.10 may also be used for hypothesis testing.

2.13 Thompson 1963: Model Formulation and Formal Testing

Kinsella (1986) formulates a model for un-replicated observations for a method comparison study as a mixed model.

$$\begin{aligned} Y_{ij} &= \mu_j + S_i + \epsilon_{ij} \quad i = 1, 2, \dots, n \quad j = 1, 2 \\ S &\sim N(0, \sigma_s^2) \quad \epsilon_{ij} \sim N(0, \sigma_j^2) \end{aligned} \tag{2.6}$$

As with all mixed models, the variance of each observation is the sum of all the associated variance components.

$$\begin{aligned} var(Y_{ij}) &= \sigma_s^2 + \sigma_j^2 \\ cov(Y_{i1}, Y_{i2}) &= \sigma_s^2 \end{aligned} \quad (2.7)$$

As with all mixed models, the variance of each observation is the sum of all the associated variance components.

$$\begin{aligned} var(Y_{ij}) &= \sigma_s^2 + \sigma_j^2 \\ cov(Y_{i1}, Y_{i2}) &= \sigma_s^2 \end{aligned} \quad (2.8)$$

Grubbs (1948) offers maximum likelihood estimators, commonly known as Grubbs estimators, for the various variance components:

$$\begin{aligned} \hat{\sigma}_s^2 &= \sum \frac{(x_i - \bar{x})(y_i - \bar{y})}{n-1} = Sxy \\ \hat{\sigma}_1^2 &= \sum \frac{(x_i - \bar{x})^2}{n-1} = S^2x - Sxy \\ \hat{\sigma}_2^2 &= \sum \frac{(y_i - \bar{y})^2}{n-1} = S^2y - Sxy \end{aligned} \quad (2.9)$$

The standard error of these variance estimates are:

$$\begin{aligned} var(\sigma_1^2) &= \frac{2\sigma_1^4}{n-1} + \frac{\sigma_S^2\sigma_1^2 + \sigma_S^2\sigma_2^2 + \sigma_1^2\sigma_2^2}{n-1} \\ var(\sigma_2^2) &= \frac{2\sigma_2^4}{n-1} + \frac{\sigma_S^2\sigma_1^2 + \sigma_S^2\sigma_2^2 + \sigma_1^2\sigma_2^2}{n-1} \end{aligned} \quad (2.10)$$

Kinsella (1986) demonstrates the estimation of the variance terms and relative precisions relevant to a method comparison study, with attendant confidence intervals for both. The measurement model introduced by Grubbs (1948, 1973) provides a formal procedure for estimating the variances σ^2 , σ_1^2 and σ_2^2 . Grubbs (1948) offers estimates, commonly known as Grubbs estimators, for the various variance components. These

estimates are maximum likelihood estimates, which shall be revisited in due course.

$$\begin{aligned}\hat{\sigma}^2 &= \sum \frac{(x_i - \bar{x})(y_i - \bar{y})}{n-1} = S_{xy} \\ \hat{\sigma}_1^2 &= \sum \frac{(x_i - \bar{x})^2}{n-1} = S^2x - S_{xy} \\ \hat{\sigma}_2^2 &= \sum \frac{(y_i - \bar{y})^2}{n-1} = S^2y - S_{xy}\end{aligned}$$

The inter-method bias is the difference of the two fixed effect terms, $\beta_1 - \beta_2$.

Kinsella (1986) demonstrates how the Grubbs estimators for the error variances can be calculated using the difference values, providing a worked example on a data set.

$$\begin{aligned}\hat{\sigma}_1^2 &= \sum (y_{i1} - \bar{y}_1)(D_i - \bar{D}) \\ \hat{\sigma}_2^2 &= \sum (y_{i2} - \bar{y}_2)(D_i - \bar{D})\end{aligned}\tag{2.11}$$

Thompson (1963) presents confidence intervals for the relative precisions of the measurement methods, $\Delta_j = \sigma_S^2/\sigma_j^2$ (where $j = 1, 2$), as well as the variances σ_S^2, σ_1^2 and σ_2^2 .

$$\Delta_1 > \frac{C_{xy} - t(|A|/n-2))^{\frac{1}{2}}}{C_x - C_{xy} + t(|A|/n-2))^{\frac{1}{2}}}\tag{2.12}$$

where

$$\begin{aligned}C_x &= (n-1)S_x^2 \\ C_{xy} &= (n-1)S_{xy} \\ C_y &= (n-1)S_y^2 \\ A &= C_x \times C_y - (C_{xy})^2\end{aligned}$$

t is the $100(1 - \alpha/2)\%$ quantile of Student's t distribution with $n - 2$ degrees of freedom. Δ_2 can be found by changing C_y for C_x . A lower confidence limit can be found by calculating the square root. This inequality may also be used for hypothesis testing.

Thompson (1963) presents three relations that hold simultaneously with probability $1 - 2\alpha$ where $2\alpha = 0.01$ or 0.05 . Thompson (1963) contains tables for K and M .

$$\begin{aligned} |\sigma^2 - C_{xy}K| &\leq M(C_x C_y)^{\frac{1}{2}} \\ |\sigma_1^2 - (C_x - C_{xy})K| &\leq M(C_x(C_x + C_y - 2C_{xy}))^{\frac{1}{2}} \\ |\sigma_2^2 - (C_y - C_{xy})K| &\leq M(C_y(C_x + C_y - 2C_{xy}))^{\frac{1}{2}} \end{aligned} \tag{2.13}$$

2.14 Structural Equation Modelling

Structural Equation modelling is a statistical technique used for testing and estimating causal relationships using a combination of statistical data and qualitative causal assumptions. Carrasco (2004) describes the structural equation model is a regression approach that allows to estimate a linear regression when independent variables are measured with error. The structural equations approach avoids the biased estimation of the slope and intercept that occurs in ordinary least square regression.

Several authors, such as Lewis et al. (1991), Kelly (1985), Voelkel and Siskowski (2005a) and Hopkins (2004) advocate the use of SEM methods for method comparison. In Hopkins (2004), a critique of the Bland-Altman plot he makes the following remark:

Authors, such as a ?, ? and Voelkel and Siskowski (2005b), strongly advocate the use of *Structural Equation Models* for the purposes of method comparison. Conversely Bland and Altman (1999) also states that consider structural equation models to be inappropriate.

What's needed for a comparison of two or more measures is a generic approach more powerful even than regression to model the relationship and error structure of each measure with a latent variable representing the true value.

Hopkins also adds that he himself is collaborating in research utilising SEM and Mixed Effects modelling. Kelly (1985) advised that *the Structural equations model is used to estimate the linear relationship between new and standards method. The Delta*

method is used to find the variance of the estimated parameters (Kelly, 1985).

However Bland and Altman (1987) contends that it is unnecessary to perform elaborate statistical analysis, while also criticizing the SEM approach on the basis that it offers insights on inter-method bias only, and not the variability about the line of equality.

However, it is quite wrong to argue solely from a lack of bias that two methods can be regarded as comparable... Knowing the data are consistent with a structural equation with a slope of 1 says something about the absence of bias but nothing about the variability about $Y = X$ (the difference between the measurements), which, as has already been stated, is all that really matters.

Chapter 3

Error In Variable Models

3.1 Background

In method comparison studies, it is of importance to assure that the presence of a difference of medical importance is detected. For a given difference, the necessary number of samples depends on the range of values and the analytical standard deviations of the methods involved. For typical examples, the present study evaluates the statistical power of least-squares and Deming regression analyses applied to the method comparison data.

3.2 Model I and II Regression

On account of the fact that one set of measurements are linearly related to another, one could surmise that Linear Regression is the most suitable approach to analyzing comparisons. This approach is unsuitable on two counts. Firstly one of the assumptions of Regression analysis is that the independent variable values are without error.

In method comparison studies one must assume the opposite; that there is error present in the measurements. Secondly a regression of X on Y would yield an entirely different result from Y on X .

Model I regression is unsuitable for method comparison studies. Even in the case

where one method is a gold standard , it is disputed as to whether it is a valid approach.

Model II regression is suitable for method comparison studies, but it is more difficult to execute. Both Model I and II regression models are unduly influenced by outliers.

Cornbleet and Cochrane (1979) argue for the use of methods that based on the assumption that both methods are imprecisely measured ,and that yield a fitting that is consistent with both ' X on Y ' and ' Y on X ' formulations. These methods uses alternatives to the OLS approach to determine the slope and intercept.

They describe three such alternative methods of regression; Deming, Mandel, and Bartlett regression. Collectively the authors refer to these approaches as Model II regression techniques.

- The authors make the distinction between model I and model II regression types.
- Model II regression is the appropriate type when the predictor variable x is measured with imprecision. Cornbleet and Cochrane remark that clinical laboratory measurements usually increase in absolute imprecision when larger values are measured.
- Model II regression is the appropriate type when the predictor variable x is measured with imprecision. Cornbleet and Cochrane remark that clinical laboratory measurements usually increase in absolute imprecision when larger values are measured.

3.2.1 Model I regression [Criterion v Test]

Cornbleet and Cochrane (1979) define this analysis as the case in which the independent variable, X , is measured without error, with y as the dependent variable.

Simple Linear Regression is well known statistical technique, wherein estimates for slope and intercept of the line of best fit are derived according to the Ordinary Least Square (OLS) principle. This method is known to Cornbleet and Cochrane (1979) as Model I regression.

Simple linear regression is defined as such with the name ‘Model I regression’ by Cornbleet and Cochrane (1979), in contrast to ‘Model II regression’.

3.2.2 Model II regression [Test V Test]

In this type of analysis, both of the measurement methods are test methods, with both expected to be subject to error. Deming regression is an approach to model II regression.

In Model I regression, the independent variable is assumed to be measured without error. For method comparison studies, both sets of measurement must be assumed to be measured with imprecision and neither case can be taken to be a reference method. Arbitrarily selecting either method as the reference will yield two conflicting outcomes. A fitting based on ‘ X on Y ’ will give inconsistent results with a fitting based on ‘ Y on X ’. Consequently model I regression is inappropriate for such cases.

Simple linear regression calculates a line of best fit for two sets of data, in which the independent variable, X , is measured without error, with y as the dependent variable.

SLR (Model I) regression is considered by many Altman and Bland (1983); Cornbleet and Cochrane (1979); Ludbrook (1997) to be wholly unsuitable for method comparison studies, although recommended for use in calibration studies [Corncoch]. Even in the case where one method is a gold standard, it is disputed as to whether it is a valid approach. Model II regression is more suitable for method comparison studies, but it is more difficult to execute. Both Model I and II regression models are unduly influenced by outliers. Regression Models can not be used to analyze repeated measurements

Conversely, Cornbleet and Cochrane (1979) state that when the independent variable X is a precisely measured reference method, Model I regression may be considered suitable. They qualify this statement by referring the X as *the correct value*, tacitly implying that there must still be some measurement error present. The validity of this approach has been disputed elsewhere.

This regression method also calculates a line of best fit for two sets of data. It differs from Model I regression in that it is derived in a way that factors in for error in the x-axis, as well as the y-axis. Cornbleet and Cochrane (1979) refer to it as 'Model II regression'.

Model II regression method also calculates a line of best fit for two sets of data. It differs from Model I regression in that it is derived in a way that factors in for error in the x-axis, as well as the y-axis. Cornbleet and Cochrane (1979) refer to it as 'Model II regression'.

- Model II regression [Test V Test] In this type of analysis, both of the measurement methods are test methods, with both expected to be subject to error. Deming regression is an approach to model II regression.
- Model I regression [Criterion v Test] Cornbleet and Cochrane (1979) define this analysis as the case in which the independent variable, X , is measured without error, with Y as the dependent variable.
- In method comparison studies, the X variable is a precisely measured reference method. In the Cornbleet and Cochrane (1979) paper It is argued that criterion may be regarded as the correct value. Other papers dispute this.

3.2.3 Contention

Several papers have commented that this approach is undermined when the basic assumptions underlying linear regression are not met, the regression equation, and consequently the estimations of bias are undermined. Outliers are a source of error in regression estimates.

In method comparison studies, the X variable is a precisely measured reference method. In the Cornbleet and Cochrane (1979) paper. It is argued that criterion may be regarded as the correct value. Other papers dispute this.

3.3 Deming Regression

The appropriate estimates were derived by Kummel (1879), but were popularized in the context of medical statistics and clinical chemistry by Deming (1943).

3.4 Error-In-Variable Models for Regression

3.4.1 Computational Aspects of Deming Regression

As stated previously, the fundamental flaw of simple linear regression is that it allows for measurement error in one variable only. This causes a downward biased slope estimate.

3.4.2 Variance Ratio

The Deming regression line is estimated by minimizing the sums of squared deviations in both the x and y directions at an angle determined by the ratio of the analytical standard deviations for the two methods.

In cases involving only single measurements by each method, λ may be unknown and is therefore assumed a value of one. While this will bias the estimates, it is less biased than ordinary linear regression.

This ratio can be estimated if multiple measurements were taken with each method, but if only one measurement was taken with each method, it can be assumed to be equal to one.

3.4.3 Estimating the Variance ratio

$$x_i = \mu + \beta_0 + \epsilon_{xi}$$

$$y_i = \mu + \beta_1 + \epsilon_{yi}$$

The inter-method bias is the difference of these biases. In order to determine an estimate for the residual variances, one of the method biases must be assumed to be zero, i.e. $\beta_0 = 0$. The inter-method bias is now represented by β_1 .

$$\begin{aligned}x_i &= \mu + \epsilon_{xi} \\y_i &= \mu + \beta_1 + \epsilon_{yi}\end{aligned}$$

The residuals can be expressed as

$$\begin{aligned}\epsilon_{xi} &= x_i - \mu \\ \epsilon_{yi} &= y_i - (\mu + \beta_1)\end{aligned}$$

The variance of the residuals are equivalent to the variance of the corresponding observations, $\sigma_{\epsilon x}^2 = \sigma_x^2$ and $\sigma_{\epsilon y}^2 = \sigma_y^2$.

$$\lambda = \frac{\sigma_{yx}^2}{\sigma_y^2}. \quad (3.1)$$

Assuming constant standard deviations, and given duplicate measurements, the analytical standard deviations are given by

$$\begin{aligned}SD_{ax}^2 &= \frac{1}{2n} \sum (x_{2i} - x_{1i})^2 \\ SD_{ay}^2 &= \frac{1}{2n} \sum (y_{2i} - y_{1i})^2\end{aligned}$$

Using duplicate measurements, one can estimate the analytical standard deviations and compute their ratio. This ratio is then used for computing the slope by the Deming method.[Linnet]

3.4.4 Inferences for Deming Regression

The Intercept and Slope are calculated according to Combleet & Gochman, 1979. The standard errors and confidence intervals are estimated using the jackknife method (Armitage et al., 2002).

The 95% confidence interval for the Intercept can be used to test the hypothesis that $A=0$. This hypothesis is accepted if the confidence interval for A contains the value 0. If the hypothesis is rejected, then it is concluded that A is significantly different from 0 and both methods differ at least by a constant amount.

The 95% confidence interval for the Slope can be used to test the hypothesis that $B=1$. This hypothesis is accepted if the confidence interval for B contains the value 1. If the hypothesis is rejected, then it is concluded that B is significantly different from 1 and there is at least a proportional difference between the two methods.

3.4.5 Expanding the use of Deming Regression for MCS

As noted before, Deming regression is an important and informative methodology in method comparison studies. For single measurement method comparisons, Deming regression offers a useful complement to LME models.

3.5 Performance in the presence of outliers

All least square estimation methods are sensitive to outliers. In common with all regression methods, Deming regression is vulnerable to outliers.

Bland Altman's 1986 paper contains a data set, measurement of mean velocity of circumferential fibre shortening (VCF) by the long axis and short axis in M-mode echocardiography. Evident in this data set are outliers. Choosing the most noticeable, we shall use the deming regression method on this data set, both with and without this outlier, to assess its influence.

- In the presence of the outlier, the intercept and slope are estimated to be -0.0297027

and 1.0172959 respectively.

- Without the outlier the intercept and slope are estimated to be -0.11482220 and 1.09263112 respectively.
- We therefore conclude that Deming Regression is adversely affected by outliers , in the same way model I regression is.

3.6 Using LME models to estimate the ratio (BXC)

$$y_{mi} = \mu + \beta_m + b_i + \epsilon_{mi}$$

with β_m is a fixed effect for the method m and b_i is a random effect associated with patient i , and ϵ_{mi} as the measurement error. This is a simple single level LME model. Pinheiro and Bates (1994) provides for the implementation of fitting a model. The variance ratio of the residual variances is immediately determinable from the output. This variance ratio can be use to fit a Deming regression, as described in chapter 1.

3.7 Linnet - References

The statistical procedures are described in: Linnet K. Necessary sample size for method comparison studies based on regression analysis. Clin Chem 1999; 45: 882-94. Linnet K. Performance of Deming regression analysis in case of misspecified analytical error ratio in method comparison studies. Clin Chem 1998; 44: 1024-1031. Linnet K. Evaluation of regression procedures for methods comparison studies. Clin Chem 1993; 39. 424-432. Linnet K. Estimation of the linear relationship between measurements of two methods with proportional errors. Stat Med 1990; 9: 1463-1473.

3.8 Ordinary Least Product Regression

Ludbrook (1997) states that the grouping structure can be straightforward, but there are more complex data sets that have a hierarchical(nested) model.

Observations between groups are independent, but observations within each groups are dependent because they belong to the same subpopulation. Therefore there are two sources of variation: between-group and within-group variance.

3.9 Least Products Regression

Used as an alternative to Bland-Altman Analysis, this method is also known as 'Geometric Mean Regression' and 'Reduced Major Axis Regression'. This regression model minimizes the areas of the right triangles formed by the data points' vertical and horizontal deviations from the fitted line and the fitted line.

Model II regression analysis caters for cases in which random error is attached to both dependent and independent variables. Comparing methods of measurement is just such a case.(Ludbrook)

Least products regression is the reviewer's preferred technique for analysing the Model II case. In this, the sum of the products of the vertical and horizontal deviations of the x,y values from the line is minimized.

Least products regression analysis is suitable for calibrating one method against another. It is also a sensitive technique for detecting and distinguishing fixed and proportional bias between methods.

Least-products regression can lead to inflated SEEs and estimates that do not tend to their true values as N approaches infinity (Draper and Smith, 1998).

Bibliography

- Altman, D. and J. Bland (1983). Measurement in medicine: The analysis of method comparison studies. *Journal of the Royal Statistical Society. Series D (The Statistician)* 32(3), 307–317.
- Altman, D. G. (1991). *Practical Statistics for Medical Research*. Chapman and Hall.
- Bartko, J. (1994). Measures of agreement: A single procedure. *Statistics in Medicine* 13, 737–745.
- Bland, J. and D. Altman (1986). Statistical methods for assessing agreement between two methods of clinical measurement. *The Lancet* i, 307–310.
- Bland, J. and D. Altman (1999). Measuring agreement in method comparison studies. *Statistical Methods in Medical Research* 8(2), 135–160.
- Bradley, E. L. and L. G. Blackwood (1989). Comparing paired data: A simultaneous test for means and variances. *The American Statistician* 43(4), 234–235.
- Carpenter, J. and J. Bithell (2000). Bootstrap confidence intervals: when, which, what? a practical guide for medical statisticians.
- Carrasco, J. L. (2004). Structural equation model. In *Encyclopedia of Biopharmaceutical Statistics, Second Edition*, pp. 1–7. Taylor & Francis.
- Carroll, R. and D. Ruppert (1996). The use and misuse of orthogonal regression in linear errors-in-variables models. *The American Statistician* 50(1), 1–6.

- Carstensen, B. (2004). Comparing and predicting between several methods of measurement. *Biostatistics* 5(3), 399–413.
- Carstensen, B., J. Simpson, and L. C. Gurrin (2008). Statistical models for assessing agreement in method comparison studies with replicate measurements. *The International Journal of Biostatistics* 4(1).
- Cohen, J., P. Cohen, S. West, and L. Aiken. *Applied multiple regression / correlation analysis for the behavioral sciences* (Third ed.). Laurence Erlbaum Associates.
- Cornbleet, P. J. and D. Cochrane (1979). Regression methods for assessing agreement between two methods of clinical measurement. *Journal of Clinical Chemistry* 24(2), 342–345.
- Dunn, G. (2002). *Statistical Evaluation of Measurement Error* (Second ed.). Stanford: American Mathematical Society and Digital Press.
- Grubbs, F. (1948). On estimating precision of measuring instruments and product variability. *Journal of the American Statistical Association* 43, 243–264.
- Grubbs, F. (1973). Errors of measurement, precision, accuracy and the statistical comparison of measuring instruments. *Technometrics* 15(1), 53–66.
- Hopkins, W. G. (2004). Bias in bland-altman but not regression validity analyses. *Sportscience* 8(4).
- Johnson, R. W. (2001). An introduction to the bootstrap. *Teaching Statistics* 23(2), 49–54.
- Kelly, G. E. (1985). Use of the structural equations model in assessing the reliability of a new measurement technique. *Applied Statistics*, 258–263.
- Kinsella, A. (1986). Estimating method precision. *The Statistician* 35, 421–427.

- Kummel, C. (1879). Reduction of observation equations which contain more than one observed quantity. *The Analyst* 6, 97–105.
- Lewis, P., P. Jones, J. Polak, and H. Tillitson (1991). The problem of conversion in method comparison studies. *Applied Statistics* 40, 105–112.
- Linnet, K. (1998). Performance of deming regression analysis in case of misspecified analytical error ratio in method comparison studies. *Clinical Chemistry* 44, 1024–1031.
- Linnet, K. (1999). Necessary sample size for method comparison studies based on regression analysis. *Clinical Chemistry* 45(6), 882–894.
- Ludbrook, J. (1997). Comparing methods of measurement. *Clinical and Experimental Pharmacology and Physiology* 24, 193–203.
- Ludbrook, J. (2002). Statistical techniques for comparing measurers and methods of measurement: a critical review. *Clinical and Experimental Pharmacology and Physiology* 29, 527–536.
- Morgan, W. A. (1939). A test for the significance of the difference between two variances in a sample from a normal bivariate population. *Biometrika* 31, 13–19.
- O’Brien, E., J. Petrie, W. Littler, M. de Swiet, P. L. Padfield, D. Altman, M. Bland, A. Coats, and N. Atkins (1990). The British Hypertension Society protocol for the evaluation of blood pressure measuring devices. *Journal of Hypertension* 8, 607–619.
- Pinheiro, J. and D. Bates (1994). *Mixed Effects Models in S and S plus* (2nd ed.). Reading, Massachusetts: Springer.
- Pitman, E. J. G. (1939). A note on normal correlation. *Biometrika* 31, 9–12.
- Thompson, W. (1963). Precision of simultaneous measurement procedures. *Journal of American Statistical Association* 58, 474–479.

Voelkel, J. G. and B. E. Siskowski (2005a). Center for quality and applied statistics
kate gleason college of engineering rochester institute of technology technical report
2005–3.

Voelkel, J. G. and B. E. Siskowski (2005b). Center for quality and applied statistics
kate gleason college of engineering rochester institute of technology technical report
2005–3.

Zhang, Y., S. Nitter-Hauge, H. Ihlen, K. Rootwelt, and E. Myhre (1986). Measurement
of aortic regurgitation by doppler echocardiography. *British Heart Journal* 55, 32–38.