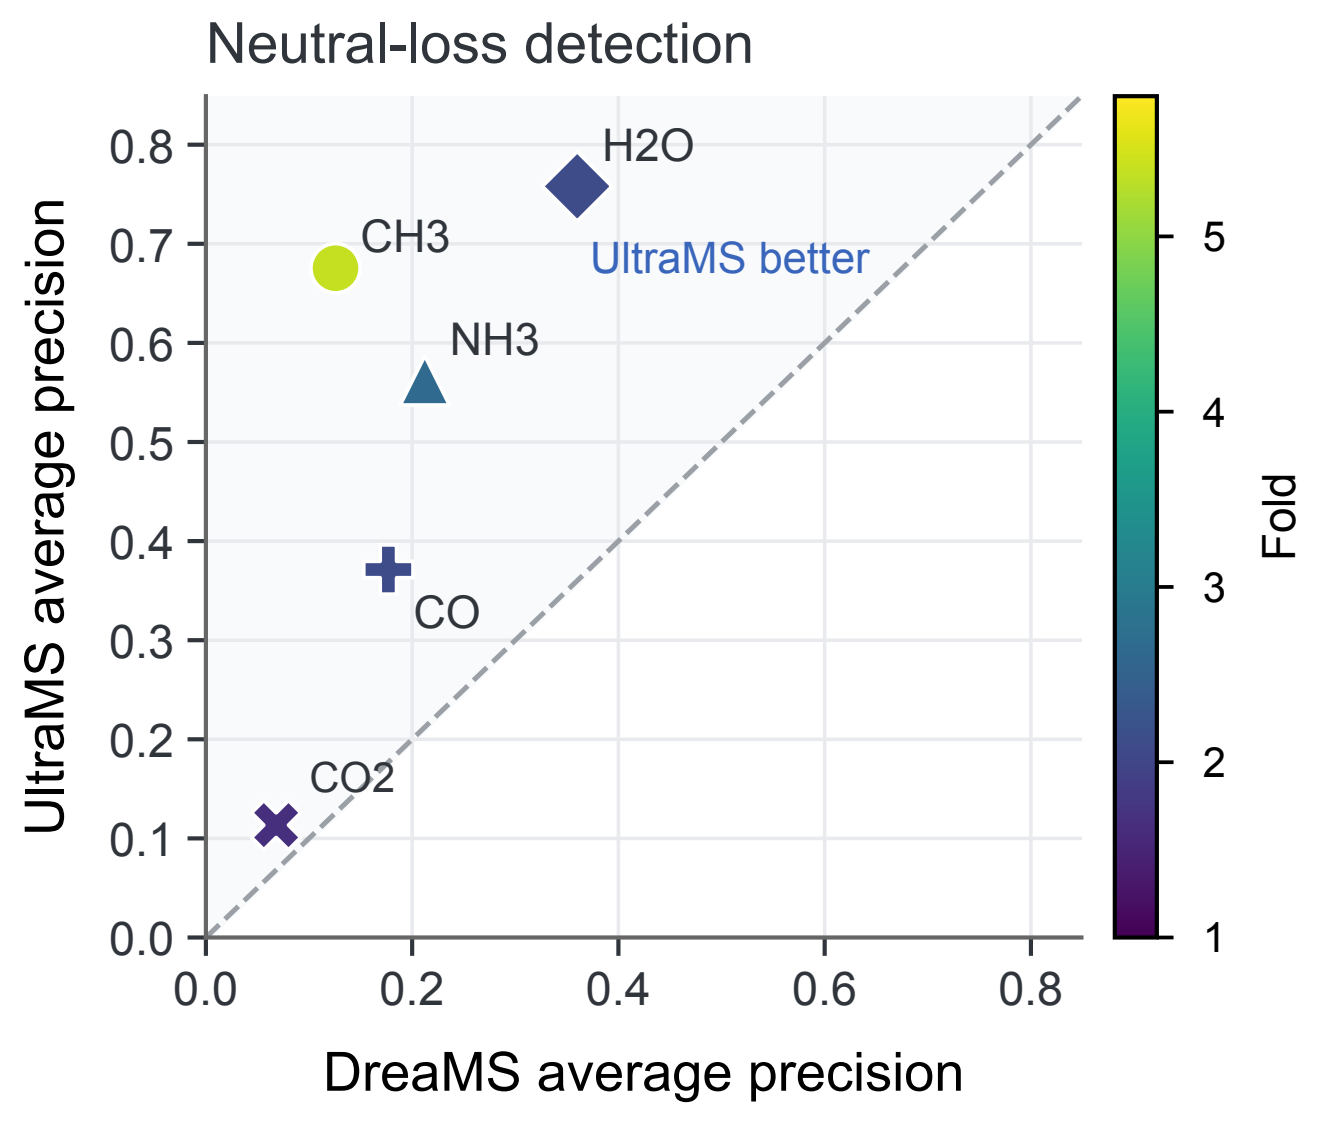
Neutral-loss detection
H2O
CH3
NH3
CO
CO2
UltraMS better
UltraMS average precision
DreaMS average precision
0.0
0.1
0.2
0.3
0.4
0.5
0.6
0.7
0.8
Fold
1
2
3
4
5