



vsázka
226103

Aut 1
Cykl 30985
program P01


spustil

31.7.2026 22:30:22

31.7.2026 23:29:30

systémová chyba není

0

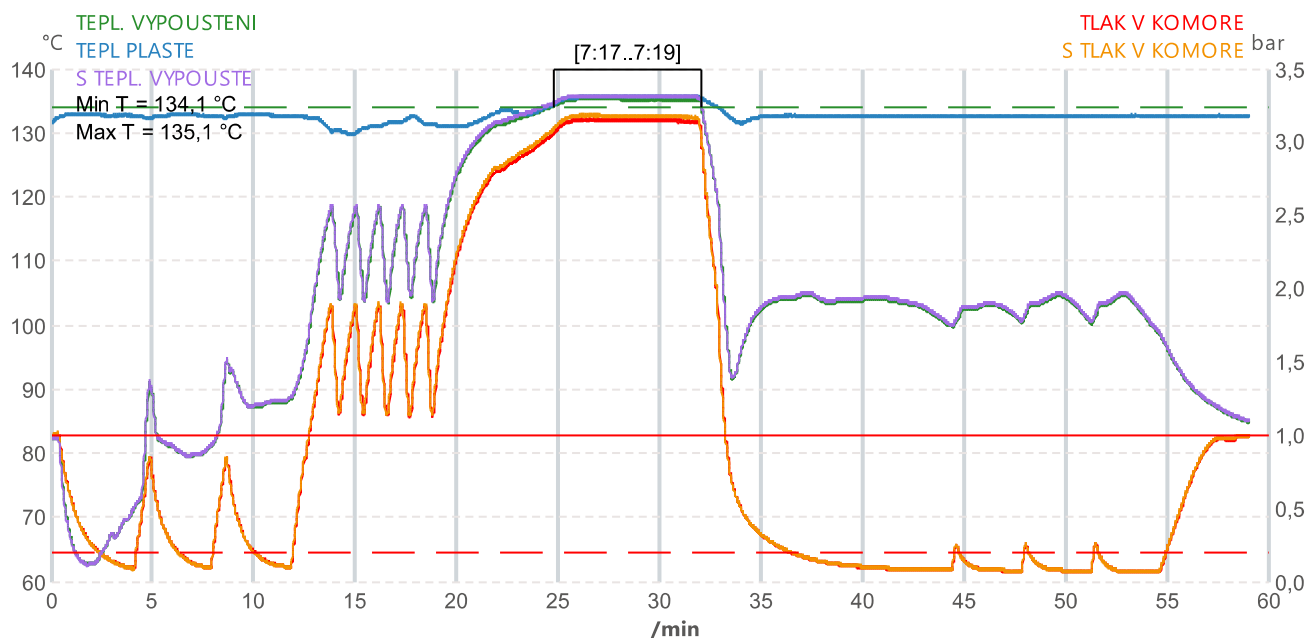

jednotky:



2110239-030-01 GSCZ PILSEN / CZECH

STRANA1

DATUM : 31/07/2026
ZACATEK PROCESU : 22:32:27
NAZEV PRISTROJE : Aut 1
CITAC CYKLU : 30985

SIGNALY
AI06 TLAK V KOMORE
AI29 S TLAK V KOMORE
AI00 TEPL. VYPOUSTENI
AI24 S TEPL. VYPOUSTE
AI01 TEPL PLASTE

PARAMETRY

NEG PULZ 3
POZ PULZ 5
TEPL STERIL 134.0 C
PREKR CAS STERIL00:07:00
CAS SUSENI 00:05:00
SUSICI PAR PULZ 00:10:00
SUSICI VZD PULZ 00:00:00

PROGRAM: P1 BALENE VYROB 134

CAS PROG	AI06	AI29	AI00	AI24	AI01
START					
00:00:00	0.978	0.985	82.1	82.2	131.4
NEG PULZACE					
00:00:15	0.996	1.001	82.1	82.3	132.0
00:01:00	0.548	0.548	66.2	66.1	132.7
00:02:00	0.248	0.247	62.6	62.5	132.6
00:03:00	0.133	0.131	67.4	67.3	132.5
00:04:00	0.083	0.081	70.8	70.9	132.5
00:04:03	0.082	0.080	71.0	71.1	132.5
NEG PULZACE					
00:04:49	0.832	0.835	90.8	91.0	132.2
00:05:00	0.706	0.704	89.1	89.2	132.2
00:06:00	0.237	0.235	80.9	81.0	132.6
00:07:00	0.117	0.115	79.5	79.6	132.6
00:07:49	0.087	0.085	80.8	81.0	132.5
00:08:00	0.222	0.222	81.3	81.4	132.5
NEG PULZACE					
00:08:36	0.819	0.825	93.1	93.3	132.2
00:09:00	0.534	0.536	92.3	92.5	132.5
00:10:00	0.194	0.192	87.1	87.2	132.7
00:11:00	0.109	0.108	87.8	88.0	132.5
00:11:46	0.091	0.090	88.3	88.5	132.5
00:12:00	0.303	0.306	89.3	89.5	132.4
POZ PULZACE					
00:12:29	0.822	0.831	94.5	94.7	132.2
00:13:00	1.242	1.253	105.2	105.5	132.1
00:13:46	1.865	1.880	117.6	118.0	130.1
00:14:00	1.459	1.458	112.6	112.9	130.1
POZ PULZACE					
00:14:13	1.146	1.154	104.0	104.2	130.1
00:15:00	1.870	1.884	117.8	118.1	129.7
POZ PULZACE					
00:15:24	1.133	1.141	103.8	104.0	130.5
00:16:00	1.769	1.781	115.8	116.2	130.7
00:16:07	1.872	1.887	117.8	118.1	130.7
POZ PULZACE					
00:16:33	1.127	1.136	103.9	104.0	131.3
00:17:00	1.654	1.666	113.7	114.0	131.6
00:17:15	1.862	1.878	117.6	117.9	131.6



POZ PULZACE

00:17:41 1.126 1.135 104.6 104.8 132.3
00:18:00 1.525 1.537 111.1 111.5 132.2
00:18:24 1.862 1.877 117.6 117.9 131.2
ZAHRIVANI

IDENTIFIKACE :Aut 1 CITAC CYKLU : 30985 STRANA2

CAS PROG AI06 AI29 AI00 AI24 AI01

00:18:49 1.123 1.132 103.9 104.1 131.2
00:19:00 1.364 1.377 107.7 107.9 131.1
00:20:00 2.203 2.221 123.0 123.4 130.7
00:21:00 2.589 2.612 128.5 128.9 131.6
00:22:00 2.793 2.817 131.1 131.5 133.1
00:23:00 2.881 2.906 132.0 132.5 132.9
00:24:00 2.969 2.996 133.1 133.5 133.1

STERILIZACE

00:24:48 3.063 3.091 134.1 134.6 134.3
00:25:18 3.118 3.146 134.8 135.2 135.1
00:25:48 3.140 3.167 135.0 135.5 135.3
00:26:18 3.144 3.172 135.1 135.6 135.4
00:26:48 3.146 3.174 135.1 135.6 135.4
00:27:18 3.144 3.172 135.1 135.5 135.4
00:27:48 3.141 3.169 135.1 135.5 135.4
00:28:18 3.139 3.167 135.0 135.5 135.4
00:28:48 3.137 3.165 135.0 135.5 135.4
00:29:18 3.138 3.166 135.0 135.5 135.4
00:29:48 3.140 3.168 135.1 135.5 135.4
00:30:18 3.137 3.165 135.0 135.5 135.5
00:30:48 3.135 3.163 135.0 135.5 135.5
00:31:18 3.131 3.159 135.0 135.4 135.5

KONECNE UPRAVY

00:31:48 3.131 3.159 135.0 135.4 135.5

NEJNIZS TEPL 134.5C

NEJVYSSI TEPL 135.1C

SUSENI

00:31:54 3.122 3.150 134.9 135.3 135.4
00:32:48 1.995 2.011 120.5 120.9 133.8
00:33:48 0.568 0.570 92.7 92.9 131.6
00:34:48 0.339 0.341 101.6 101.9 132.2
00:35:48 0.236 0.238 103.7 104.0 132.5
00:36:48 0.173 0.175 104.1 104.4 132.5
00:37:48 0.132 0.134 103.9 104.1 132.5
00:38:48 0.109 0.112 103.5 103.8 132.5
00:39:21 0.100 0.102 103.6 103.9 132.5
00:39:48 0.094 0.096 103.6 103.9 132.5
00:40:48 0.083 0.085 103.9 104.2 132.5
00:41:48 0.078 0.079 103.4 103.7 132.5
00:42:48 0.073 0.075 102.7 103.0 132.5
00:43:48 0.073 0.074 100.8 101.1 132.5

SUSICI PAR PULZ

00:44:25 0.085 0.086 99.5 99.8 132.5
00:44:48 0.173 0.174 101.8 102.1 132.5
00:45:48 0.077 0.078 102.6 102.9 132.5
00:46:48 0.068 0.068 102.5 102.9 132.5
00:47:48 0.064 0.065 100.4 100.7 132.5

SUSICI PAR PULZ

00:47:50 0.064 0.065 100.3 100.6 132.5
00:48:48 0.097 0.097 103.2 103.5 132.5



00:49:48 0.068 0.068 104.4 104.7 132.5
00:50:48 0.062 0.063 101.8 102.1 132.5
SUSICI PAR PULZ
00:51:16 0.061 0.062 100.2 100.5 132.5
00:51:48 0.144 0.144 102.9 103.2 132.4
00:52:48 0.062 0.063 104.6 104.9 132.5
00:53:48 0.058 0.059 101.6 101.9 132.5
VYROVNAVANI
00:54:37 0.057 0.058 98.5 98.8 132.5
00:54:48 0.133 0.133 97.4 97.7 132.5

IDENTIFIKACE :Aut 1 CITAC CYKLU : 30985 STRANA3

CAS PROG AI06 AI29 AI00 AI24 AI01

00:55:48 0.531 0.534 91.9 92.1 132.5
00:56:48 0.863 0.868 88.4 88.6 132.5
PROCES UKONCEN
00:57:30 0.965 0.971 86.9 87.1 132.5
PROCES OK

PODPIS: