



vsázka
226118

Aut 4
Cykl 28851
program P02


spustil

1.8.2026 20:49:45

1.8.2026 22:05:18

systémová chyba není

0

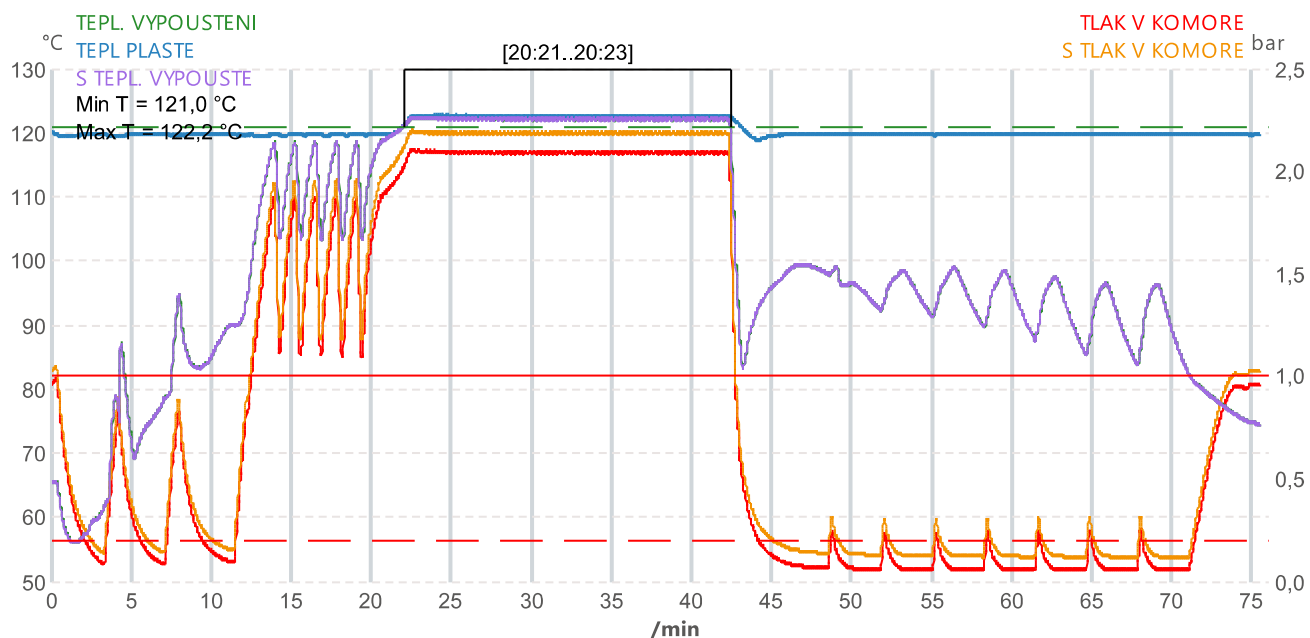

jednotky:



2110239-010-01 GSCZ PILSEN CZECH

STRANA1

DATUM : 01/08/2026
ZACATEK PROCESU : 21:38:36
NAZEV PRISTROJE : Aut 4
CITAC CYKLU : 28851

SIGNALY
AI06 TLAK V KOMORE
AI29 S TLAK V KOMORE
AI00 TEPL. VYPOUSTENI
AI24 S TEPL. VYPOUSTE
AI01 TEPL PLASTE

PARAMETRY

NEG PULZ 3
POZ PULZ 5
TEPL STERIL 121.0 C
PREKR CAS STERIL00:20:00
CAS SUSENI 00:03:00
SUSICI PAR PULZ 00:20:00
SUSICI VZD PULZ 00:00:00

PROGRAM: P2 BALENE VYROB 121

CAS PROG	AI06	AI29	AI00	AI24	AI01
START					
00:00:00	0.959	1.019	65.3	65.3	119.9
NEG PULZACE					
00:00:15	0.978	1.037	65.3	65.3	119.6
00:01:00	0.510	0.568	57.3	57.1	119.3
00:02:00	0.213	0.270	56.9	56.8	119.5
00:03:00	0.096	0.152	59.9	59.8	119.5
00:03:16	0.079	0.135	61.3	61.2	119.5
00:04:00	0.681	0.743	78.5	78.6	119.3
NEG PULZACE					
00:04:10	0.824	0.883	78.0	78.0	119.3
00:05:00	0.329	0.387	72.1	72.0	119.7
00:06:00	0.141	0.199	74.2	74.1	119.6
00:07:00	0.081	0.139	78.1	78.0	119.5
00:07:02	0.080	0.138	78.3	78.3	119.5
NEG PULZACE					
00:07:55	0.820	0.880	94.3	94.3	119.5
00:08:00	0.813	0.872	94.6	94.5	119.5
00:09:00	0.271	0.332	83.3	83.2	119.6
00:10:00	0.142	0.200	85.0	84.9	119.5
00:11:00	0.095	0.155	89.4	89.3	119.5
00:11:22	0.089	0.149	89.8	89.8	119.5
00:12:00	0.684	0.744	91.4	91.4	119.5
POZ PULZACE					
00:12:12	0.820	0.883	94.6	94.5	119.4
00:13:00	1.332	1.401	107.9	107.8	119.3
00:13:52	1.862	1.937	118.2	118.1	119.5
00:14:00	1.794	1.865	118.0	117.9	119.6
POZ PULZACE					
00:14:17	1.119	1.195	103.6	103.5	119.4
00:15:00	1.758	1.835	116.2	116.1	119.6
00:15:10	1.862	1.941	118.1	118.1	119.6
OPOZ PULZACE					
00:15:34	1.100	1.179	104.0	103.9	119.6
00:16:00	1.554	1.635	112.3	112.3	119.5
00:16:26	1.857	1.939	118.0	117.9	119.6
POZ PULZACE					
00:16:49	1.097	1.178	103.5	103.4	119.5
00:17:00	1.258	1.339	105.7	105.7	119.4



00:17:46 1.859 1.944 118.0 118.0 119.6
00:18:00 1.408 1.492 112.4 112.3 119.6
POZ PULZACE
00:18:10 1.097 1.180 103.3 103.3 119.6
00:19:01 1.858 1.944 118.0 117.9 119.6

IDENTIFIKACE :Aut 4 CITAC CYKLU : 28851 STRANA2

CAS PROG AI06 AI29 AI00 AI24 AI01

ZAHRIVANI

00:19:24 1.101 1.186 103.2 103.2 119.5
00:20:00 1.667 1.753 114.8 114.7 119.5
00:21:00 1.901 1.990 119.0 119.0 119.6
00:22:00 2.012 2.103 120.7 120.7 120.9

STERILIZACE

00:22:09 2.049 2.140 121.2 121.2 121.3
00:22:30 2.094 2.187 122.1 122.1 122.3
00:23:00 2.094 2.187 122.1 122.1 122.4
00:23:30 2.090 2.184 122.1 122.0 122.5
00:24:00 2.092 2.186 122.1 122.1 122.5
00:24:30 2.092 2.186 122.1 122.0 122.5
00:25:00 2.092 2.186 122.0 122.0 122.5
00:25:30 2.091 2.185 122.0 122.0 122.5
00:26:00 2.091 2.185 122.0 122.0 122.5
00:26:30 2.092 2.186 122.0 122.0 122.5
00:27:00 2.090 2.185 122.1 122.0 122.5
00:27:30 2.090 2.185 122.0 121.9 122.5
00:28:00 2.090 2.185 122.0 122.0 122.5
00:28:30 2.090 2.184 122.0 121.9 122.5
00:29:00 2.085 2.179 121.9 121.9 122.5
00:29:30 2.081 2.176 122.0 121.9 122.5
00:30:00 2.082 2.177 122.0 121.9 122.5
00:30:30 2.084 2.179 122.0 122.0 122.5
00:31:00 2.084 2.179 122.0 122.0 122.5
00:31:30 2.086 2.181 122.0 122.0 122.5
00:32:00 2.088 2.183 122.0 122.0 122.5
00:32:30 2.088 2.183 122.0 122.0 122.5
00:33:00 2.091 2.186 122.0 122.0 122.5
00:33:30 2.091 2.187 122.0 122.0 122.5
00:34:00 2.081 2.176 122.0 121.9 122.5
00:34:30 2.085 2.180 122.0 122.0 122.5
00:35:00 2.087 2.182 122.0 122.0 122.5
00:35:30 2.092 2.186 122.0 122.0 122.5
00:36:00 2.090 2.185 122.0 121.9 122.5
00:36:30 2.081 2.176 122.0 121.9 122.5
00:37:00 2.084 2.179 122.0 122.0 122.5
00:37:30 2.087 2.181 122.0 122.0 122.5
00:38:00 2.091 2.186 122.0 122.0 122.5
00:38:30 2.089 2.184 122.0 121.9 122.5
00:39:00 2.083 2.178 122.0 122.0 122.5
00:39:30 2.085 2.180 122.0 122.0 122.5
00:40:00 2.092 2.186 122.0 122.0 122.5
00:40:30 2.081 2.176 122.0 121.9 122.5
00:41:00 2.085 2.180 122.0 122.0 122.5
00:41:30 2.090 2.185 122.1 122.0 122.5
00:42:00 2.081 2.176 121.9 121.9 122.5

KONECNE UPRAVY

00:42:09 2.086 2.181 122.0 122.0 122.5

NEJNIZS TEPL 121.9C



NEJVYSSI TEPL 122.2C

SUSENI

00:42:15	2.081	2.176	122.0	121.9	122.4
00:43:00	0.584	0.666	87.6	87.5	121.0
00:44:00	0.219	0.300	91.7	91.6	118.8
00:45:00	0.121	0.201	95.6	95.6	119.3
00:45:27	0.099	0.178	96.8	96.8	119.5
00:46:00	0.081	0.159	98.1	98.1	119.5
00:47:00	0.066	0.143	99.2	99.1	119.5
00:48:00	0.060	0.135	98.4	98.4	119.5

IDENTIFIKACE :Aut 4

CITAC CYKLU : 28851

STRANA3

CAS PROG AI06 AI29 AI00 AI24 AI01

SUSICI PAR PULZ

00:48:32	0.059	0.133	97.8	97.8	119.5
00:49:00	0.147	0.220	98.8	98.8	119.5
00:50:00	0.059	0.130	96.3	96.4	119.5
00:51:00	0.054	0.125	94.3	94.3	119.5

SUSICI PAR PULZ

00:51:49	0.052	0.122	92.1	92.1	119.5
00:52:00	0.227	0.298	93.5	93.5	119.5
00:53:00	0.059	0.127	98.0	98.0	119.5
00:54:00	0.053	0.121	95.2	95.2	119.5
00:55:00	0.050	0.118	91.2	91.2	119.5

SUSICI PAR PULZ

00:55:02	0.050	0.118	91.1	91.1	119.5
00:56:00	0.069	0.136	97.6	97.6	119.6
00:57:00	0.052	0.118	95.7	95.7	119.5
00:58:00	0.050	0.117	90.4	90.4	119.5

SUSICI PAR PULZ

00:58:14	0.050	0.116	89.5	89.5	119.5
00:59:00	0.090	0.155	96.2	96.2	119.5
01:00:00	0.053	0.117	95.9	95.9	119.5
01:01:00	0.050	0.115	89.7	89.7	119.5

SUSICI PAR PULZ

01:01:26	0.059	0.127	87.5	87.5	119.5
01:02:00	0.117	0.181	94.3	94.3	119.5
01:03:00	0.053	0.117	95.8	95.9	119.5
01:04:00	0.051	0.114	88.6	88.6	119.5

SUSICI PAR PULZ

01:04:37	0.055	0.120	85.2	85.2	119.5
01:05:00	0.181	0.244	90.0	90.1	119.5
01:06:00	0.054	0.117	96.0	96.0	119.5
01:07:00	0.051	0.114	88.4	88.4	119.5

SUSICI PAR PULZ

01:07:48	0.054	0.116	83.5	83.5	119.5
01:08:00	0.236	0.301	85.7	85.7	119.5
01:09:00	0.056	0.118	96.1	96.1	119.5
01:10:00	0.052	0.113	89.0	89.0	119.5

VYROVNAVANI

01:11:00	0.051	0.112	82.4	82.3	119.5
01:12:00	0.446	0.509	79.6	79.6	119.5
01:13:00	0.800	0.864	77.5	77.5	119.5

PROCES UKONCEN

01:13:54	0.944	1.008	75.9	75.9	119.5
----------	-------	-------	------	------	-------

PROCES OK



PODPIS: