## Optimal acquisition scheme for subwavelength localization microscopy of bleachable fluorophores: erratum

## Edward Shore<sup>1</sup> and Alex Small<sup>2,\*</sup>

<sup>1</sup>Mathematics and Statistics Department, California State Polytechnic University, 3801 West Temple Avenue, Pomona, California 91768, USA

<sup>2</sup>Physics Department, California State Polytechnic University, 3801 West Temple Avenue, Pomona, California 91768, USA

 $*Corresponding\ author:\ arsmall@csupomona.edu$ 

Received July 11, 2011; accepted July 11, 2011; posted July 11, 2011 (Doc. ID 150681); published August 8, 2011

One of the plots in Fig. 2 of our previous Letter [Opt. Lett. **36**, 289 (2011)] was mislabeled with an incorrect parameter value and is corrected here. © 2011 Optical Society of America *OCIS codes*: 180.2520, 100.6640.

In our recently published Letter [1], the third plot in Fig. 2 was incorrectly labeled. The parameter value used to generate that plot was  $f_1 = 0.5$ , not  $f_1 = 0.05$ . A corrected version of the figure is included (Fig. 1).

## References

1. E. Shore and A. Small, Opt. Lett. **36**, 289 (2011).

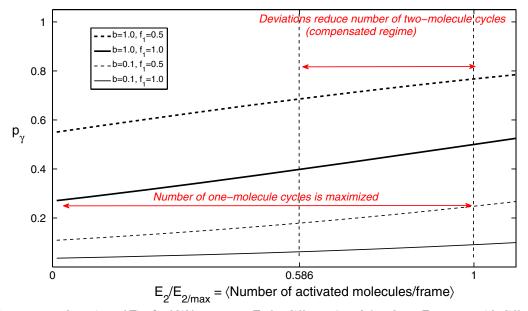


Fig. 1. (This is a corrected version of Fig. 2 of [1].)  $p_{\gamma}$  versus  $E_2$  for different b and  $f_1$  values.  $E_2$  ranges with different qualitative features are noted.