


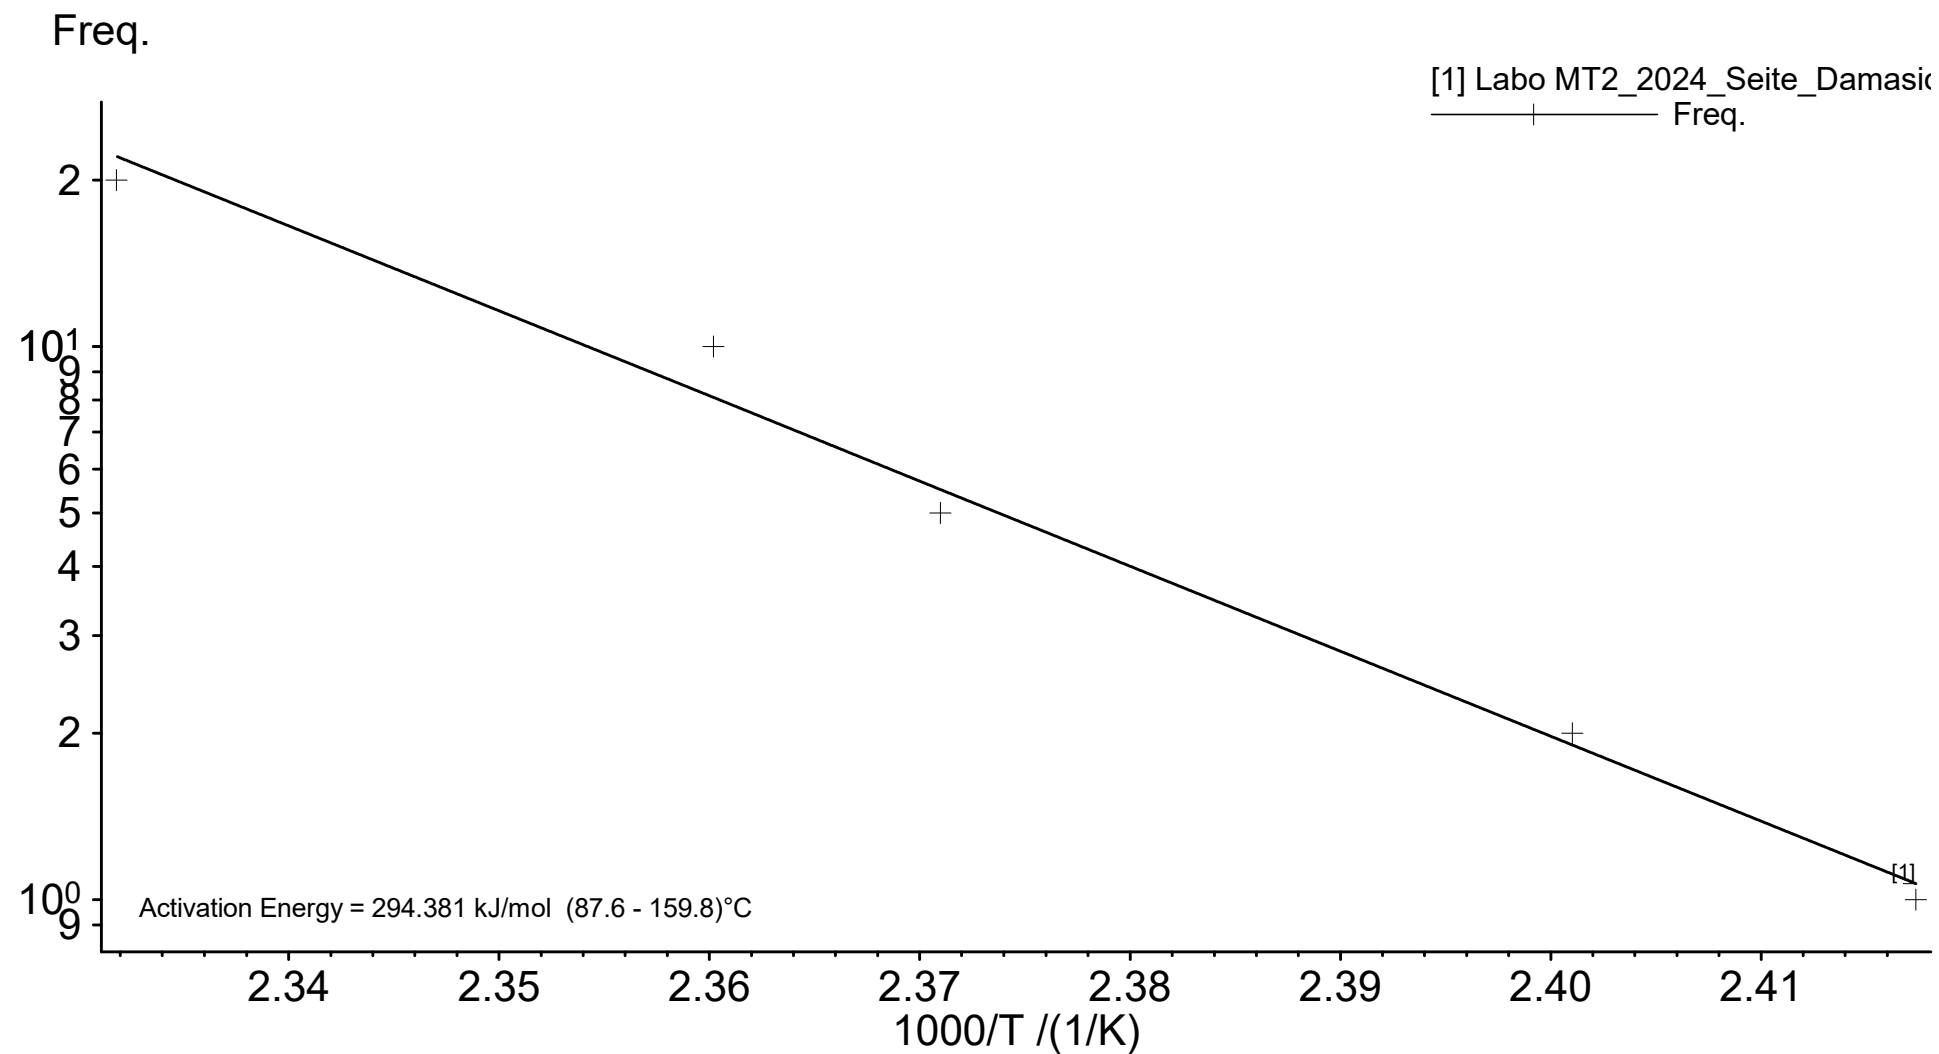

Arrhenius 2025-11-06 10:44 User: HEPIA

Instrument : NETZSCH DMA 242		File : C:\NETZSCH\Proteus61\data\Labo MT2_2024_Seite_Damasio_n°6.ngb-dm2		
Identity : EXP_00	Sample dim. : 20.000x11.000x3.000 mm	Temp. range : 70.0°C/5.0(K/min)/180.0°C	Calibration : 20240522 Dynamic Mass Calibration.mm2	
Date/time : 11/6/2025 10:00:02 AM	Deform. mode : 3pt bending 20	Segments : 1/1	Calibration : 20240522 Empty system calibration.em2	
Laboratory : Nano	Amplitude : 30.00 um	Frequency : 1Hz;2Hz;5Hz;10Hz;20Hz	Calibration : 20240522 system stiffness calib_3point bending.cm1	
Operator : mdf	DF/CSF : 3.00 N / 0.10 N	Atmosphere :	Calibration : Phasenabgleich.rm2	
Project : Test 3 pts apres calib	PF : 1.10	Flow rate : 0 ml/min	Temp.calib. : TCALZERO.TMX	
Sample/shape : PMMA/Cubic	Material : pmma	Smoothing : 3e-005/0.1 - 0		

Created with NETZSCH Proteus software