


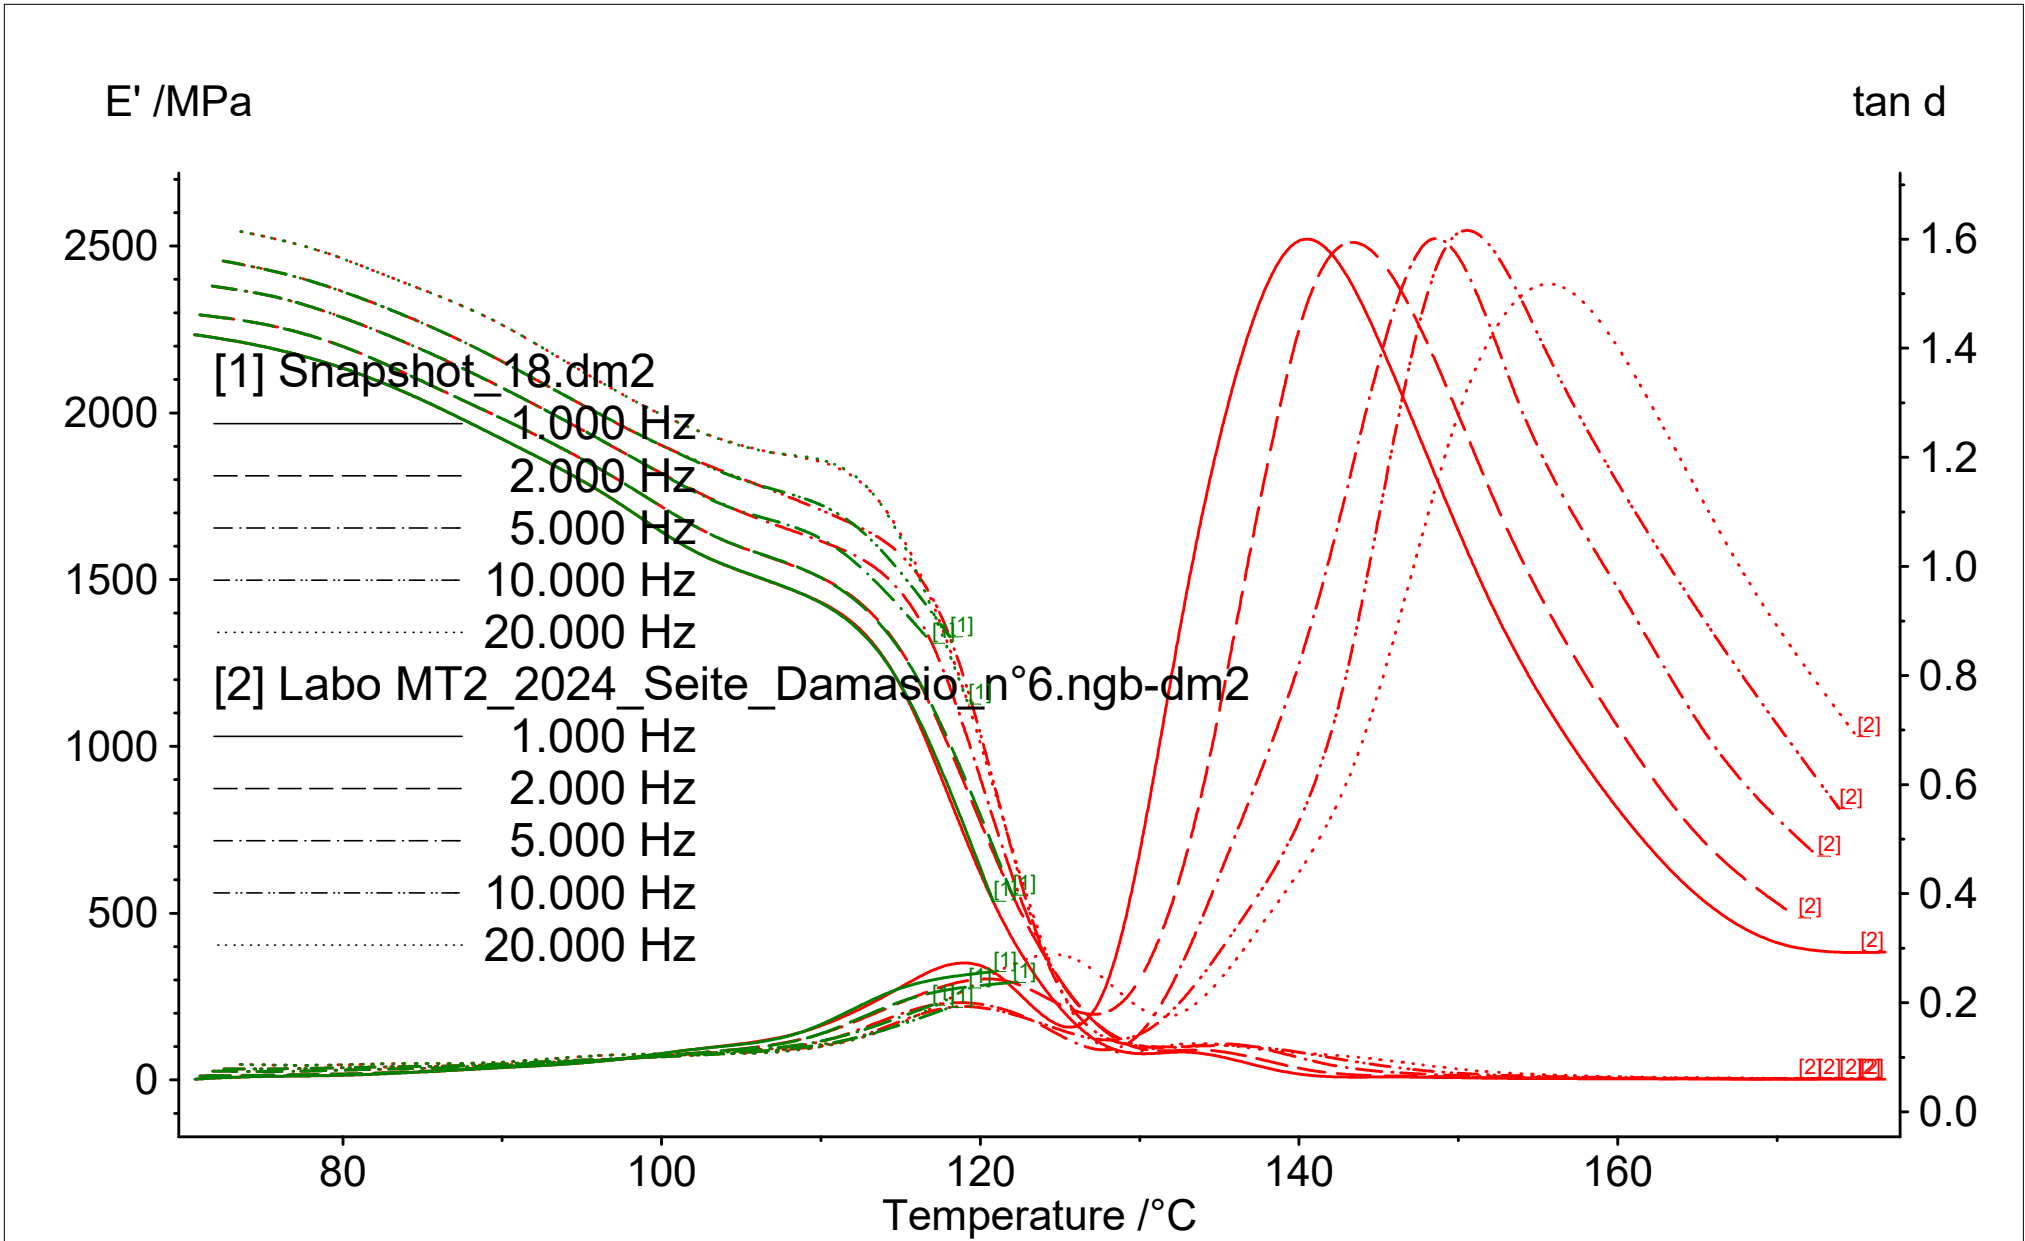

Main 2025-11-06 10:30 User: HEPIA

[#]	Instru...	File	Date	Identity	Sa...	Sample dim./mm	S...	Range	Frequen...	Calibrations	Smooth...
[1]	DMA 2...	Snapshot_18.dm2	2025-11-...	EXP_...	PM...	20.000x11.000x3.0...	1...	70.0°C/5.0(K/min)/180.0...	1;2;5;10;...	20240522 Em... .em2+20240522 sy... .c...	3e-005,...
[2]	DMA 2...	Labo MT2_2024_Seite_Damasio_n°6.ngb-d...	2025-11-...	EXP_...	PM...	20.000x11.000x3.0...	1...	70.0°C/5.0(K/min)/180.0...	1;2;5;10;...	20240522 Em... .em2+20240522 sy... .c...	3e-005,...