EIDSS | Electronic Integrated Disease Surveillance System
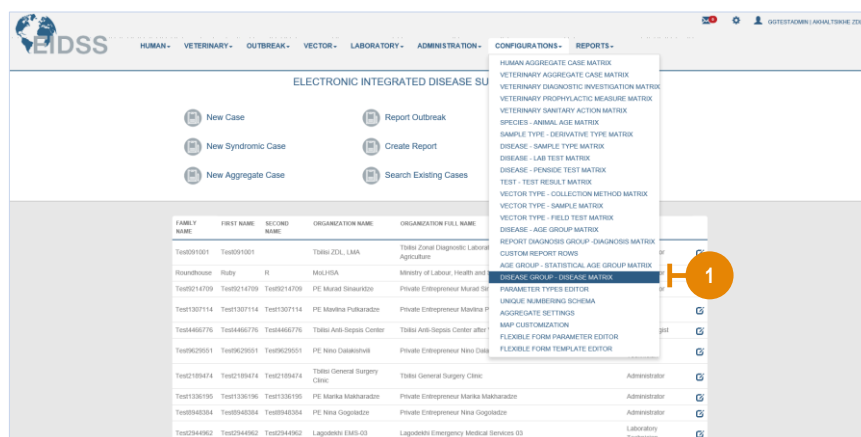
Configure the Disease Group – Disease Matrix

An EIDSS user with the appropriate permissions can specify disease associations in the database. This quick guide presents the steps to configure the Disease Group – Disease matrix.
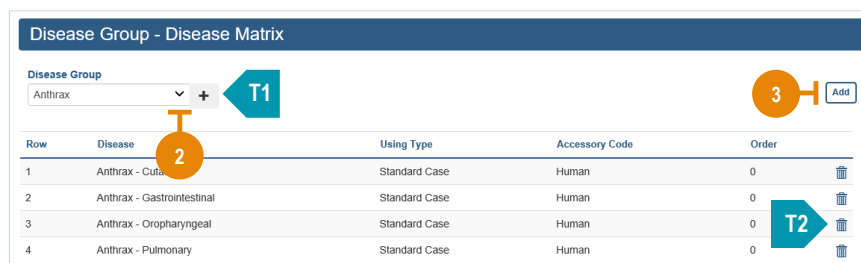
1. From the **EIDSS Dashboard,** choose **DISEASE GROUP – DISEASE MATRIX** from the **CONFIGURATIONS** drop-down menu. The **Disease Group – Disease Matrix** screen appears.

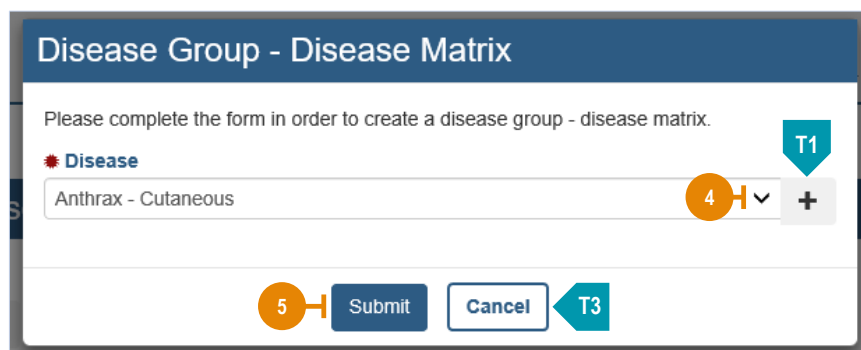2. Choose a **Disease Group** from the drop-down menu. Any existing **Diseases** appear in the grid.

> **Tip 1:** To add a new option, click the **Add** icon, complete the window that appears and click **Submit.**

> **Tip 2:** To delete a row, click the corresponding **Delete** icon and click **Yes** on the dialog box that appears.

3. Click **Add.** The **Disease Group – Disease Matrix** window appears.

4. Choose a **Disease** from the drop-down menu.

> **Tip 3:** To delete entered information and close the window, click **Cancel.**

5. Click **Submit.** A pop-up appears confirming successful configuration of the matrix. **Note:** The **Using Type** and **Accessory Code** fields auto-populate in the grid.