



Thermal ablation fails in a place, and electroporation does not fail there


(a) blood carries the heat away

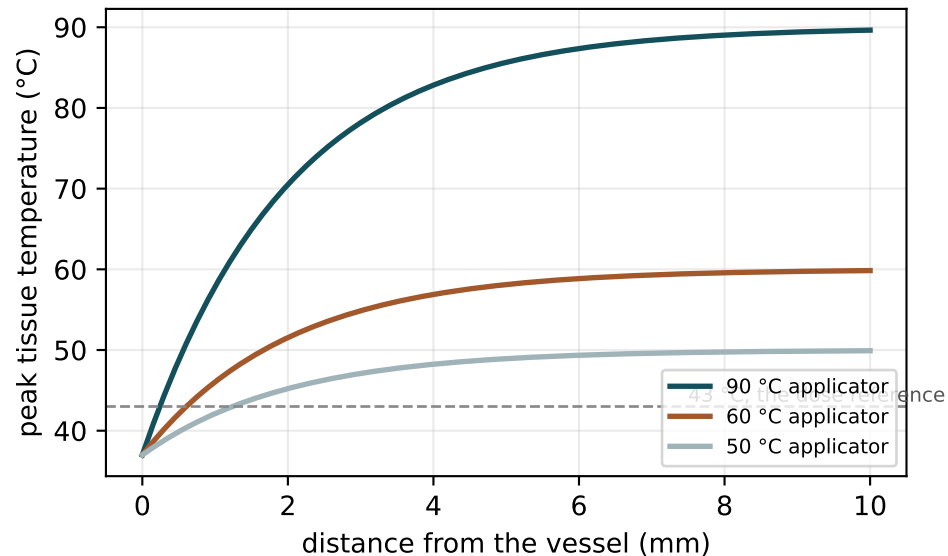

(b) a radius, not a percentage

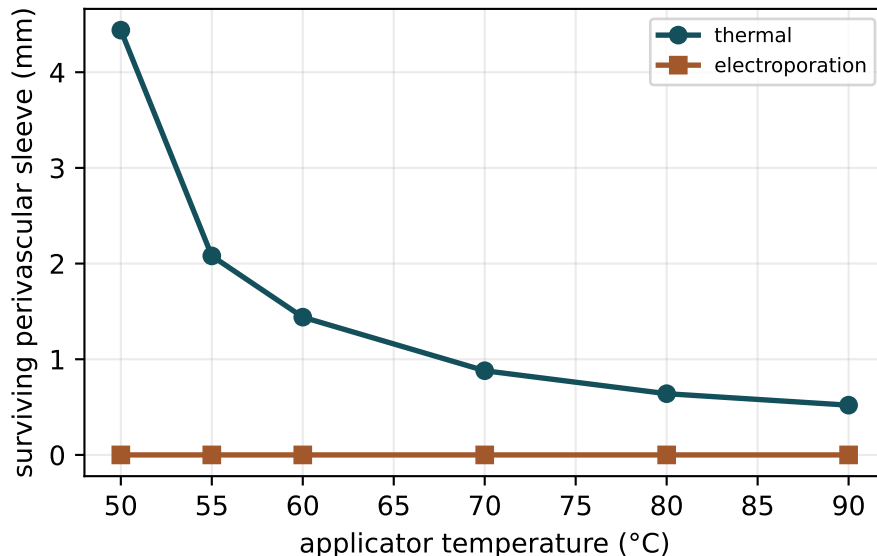

(c) the size is a restatement of an assumption

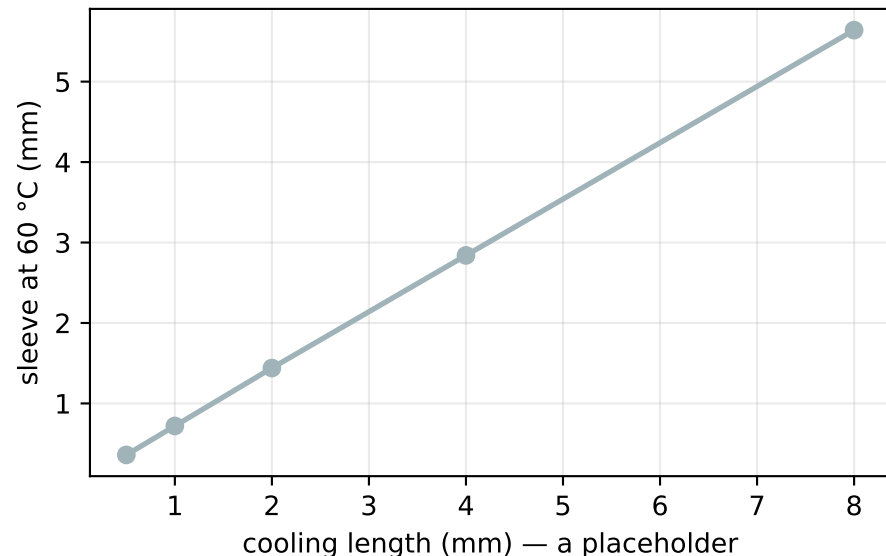

This arm's calibration is UNCONSTRAINED and will stay so: a threshold observable cannot identify a threshold parameter. What replaces it is a statement about WHERE the survivors are - a radius rather than a coverage percentage, which a clinician can look for. Electroporation's zero is structural rather than measured: it is non-thermal, so a heat sink removes nothing that matters to it, which is the documented reason it is reached for near vessels. (c) is why the SIZE is not a result: the cooling length stands in for vessel calibre and flow, which this layer does not represent, and the sleeve scales with it almost proportionally.