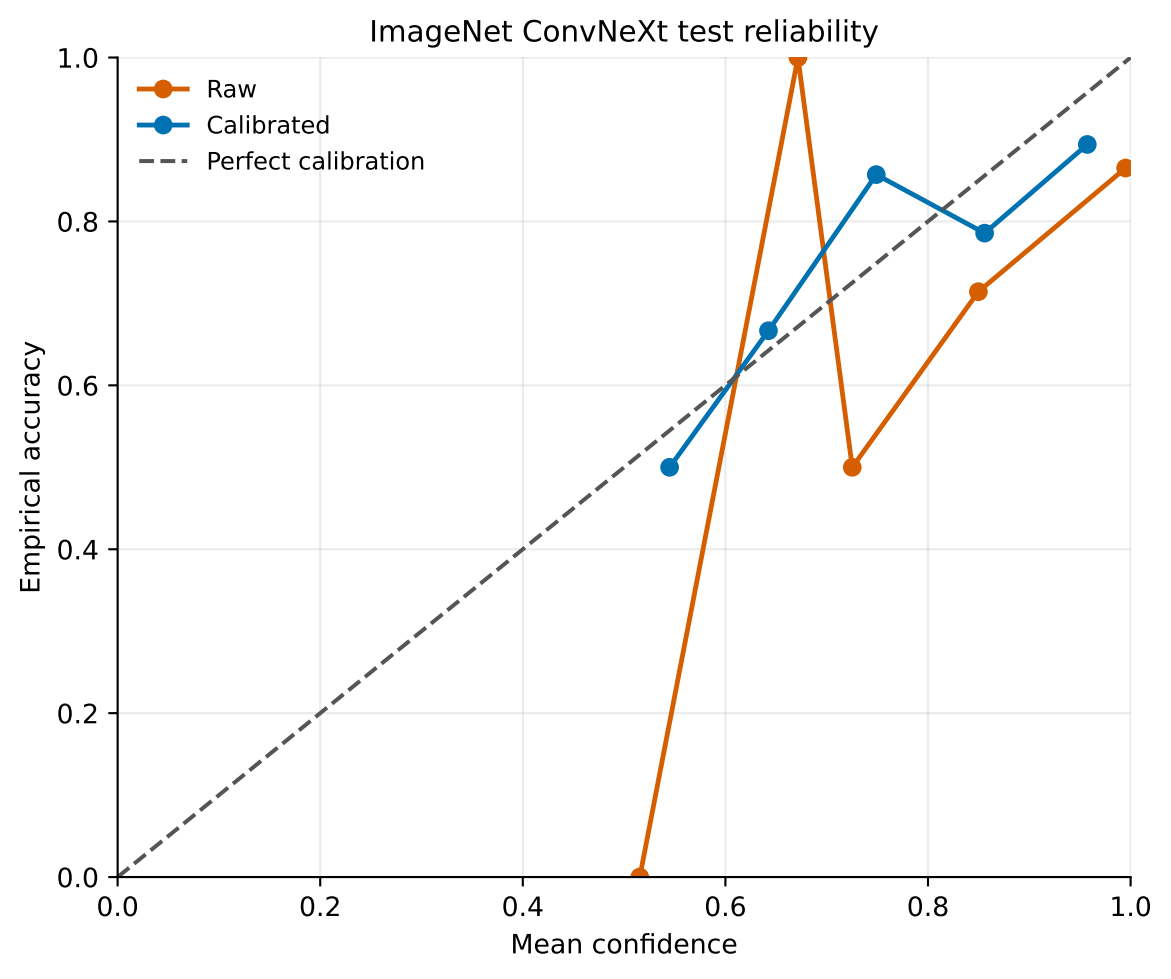
ImageNet ConvNeXt test reliability
Raw
Calibrated
Perfect calibration
Empirical accuracy
Mean confidence
0.0
0.2
0.4
0.6
0.8
1.0