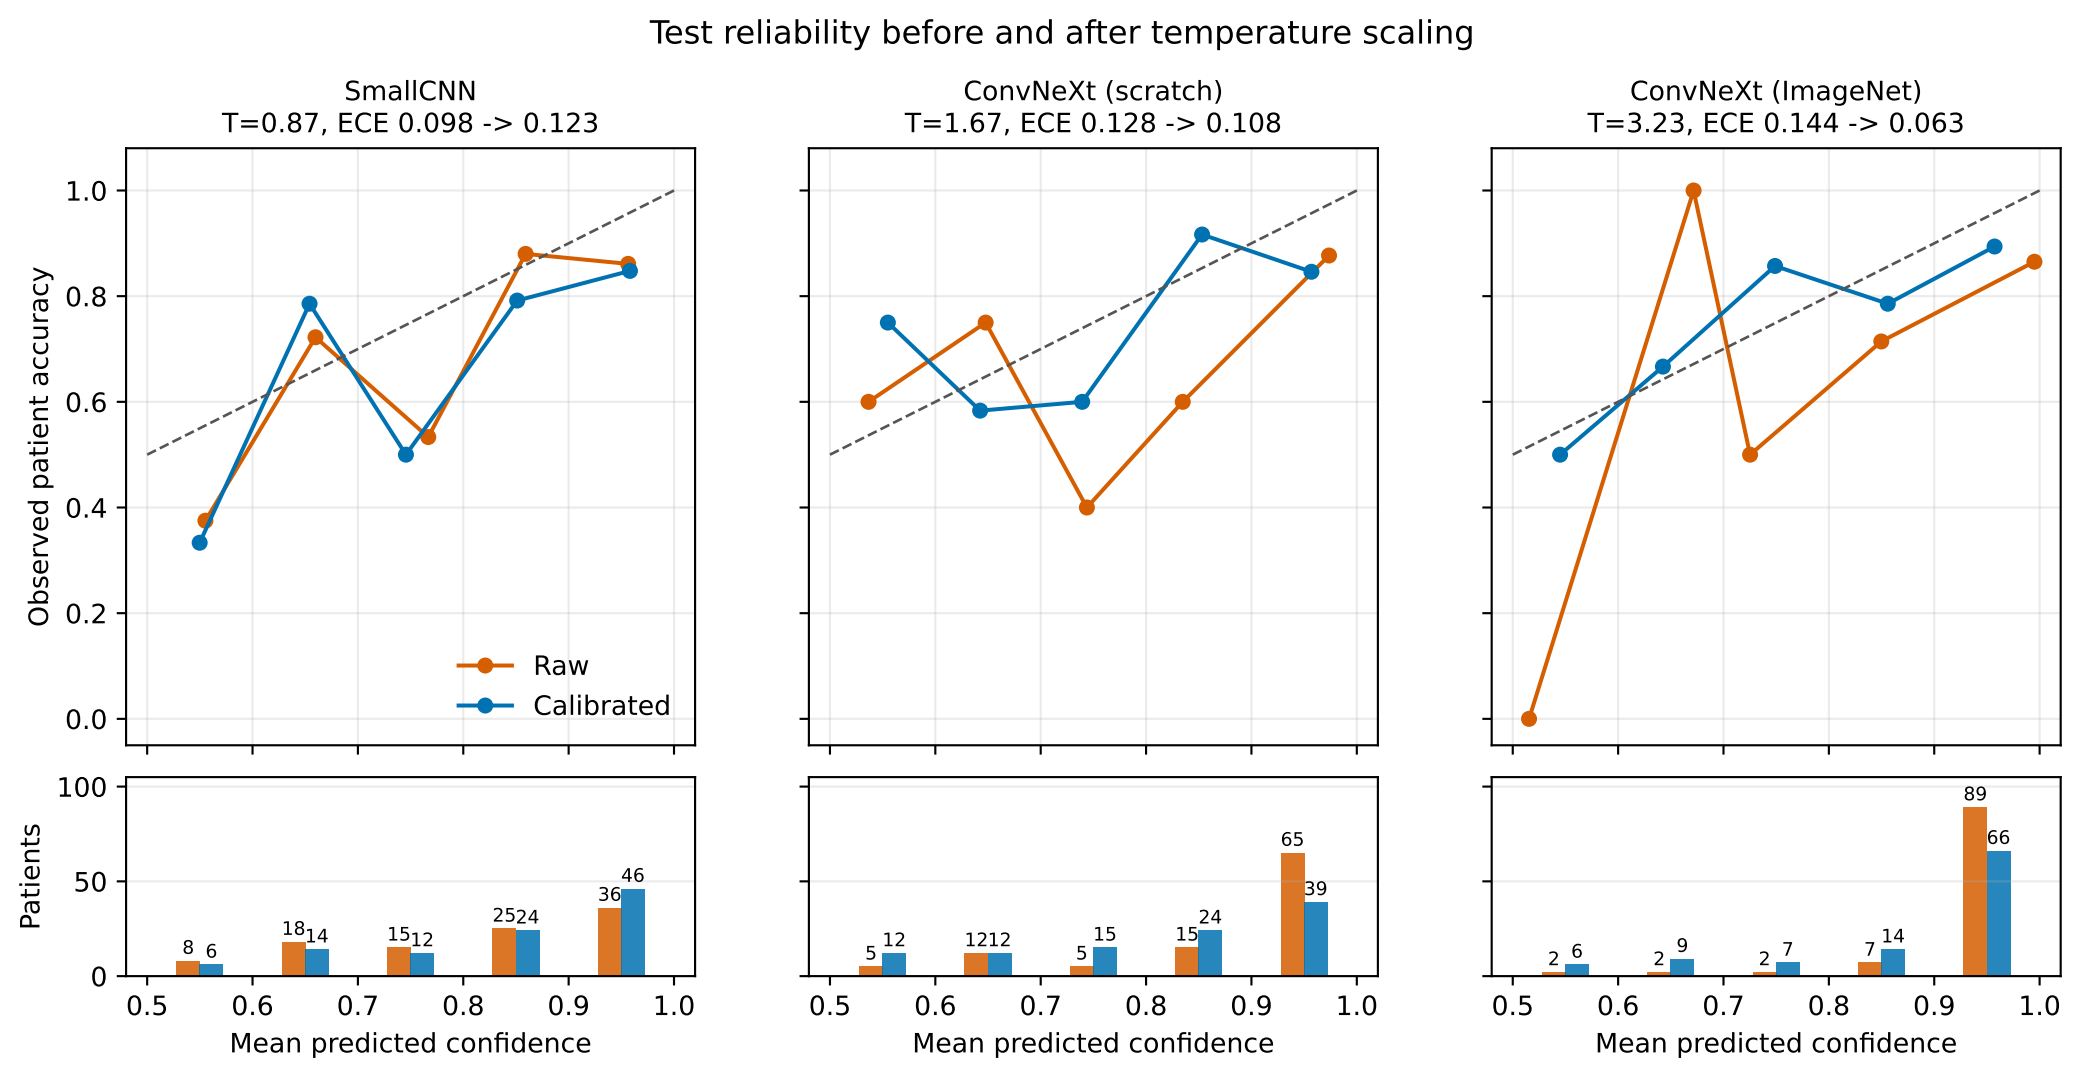
Test reliability before and after temperature scaling
SmallCNN
T=0.87, ECE 0.098 -> 0.123
ConvNeXt (scratch)
T=1.67, ECE 0.128 -> 0.108
ConvNeXt (ImageNet)
T=3.23, ECE 0.144 -> 0.063
Observed patient accuracy
Raw
Calibrated
Patients
Mean predicted confidence
Mean predicted confidence
Mean predicted confidence