

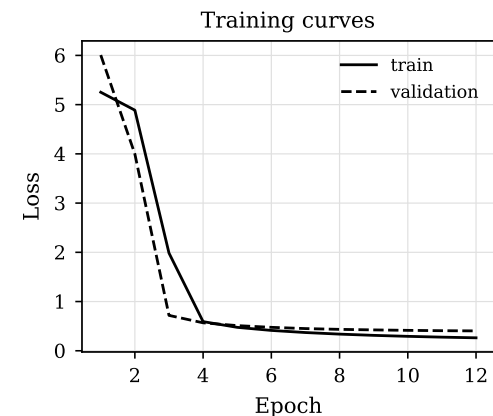
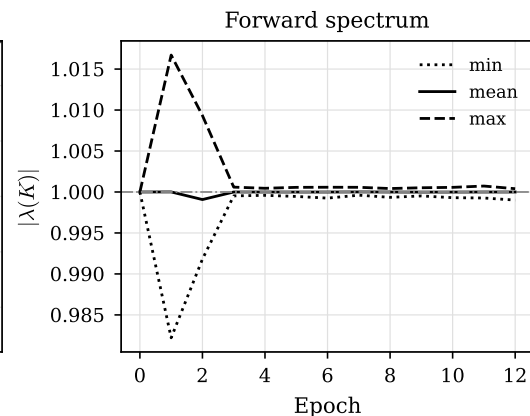
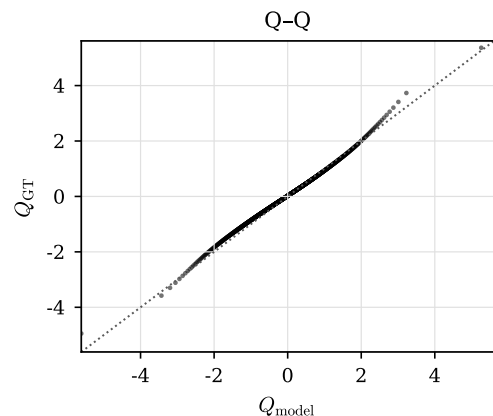
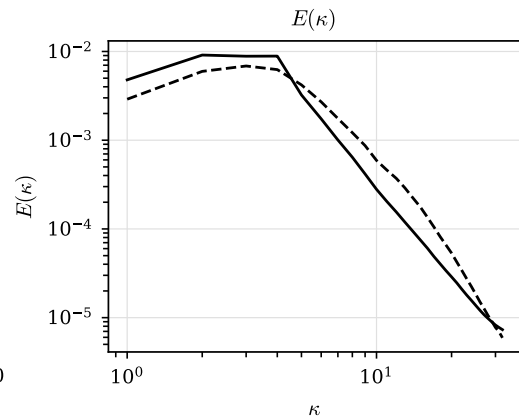
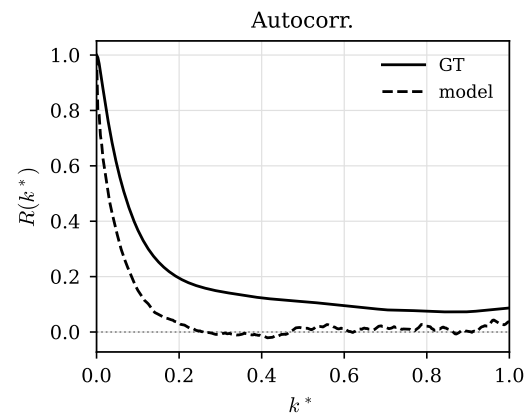
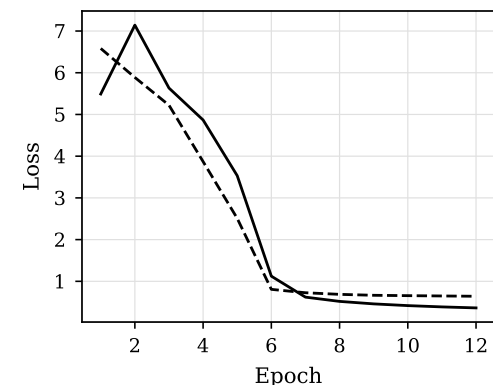
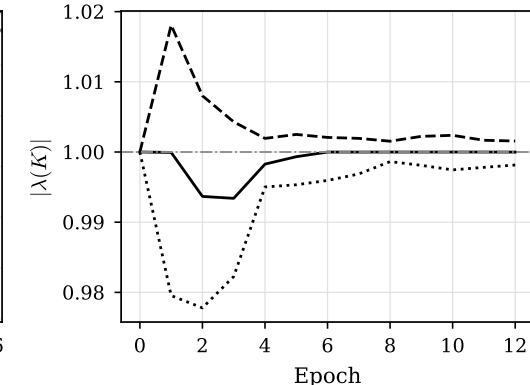
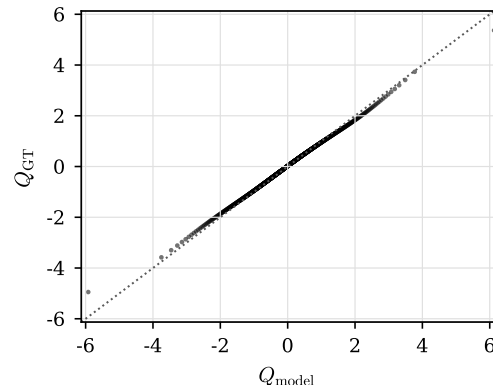


Strict single-operator AR ablations

Strict single- K baseline

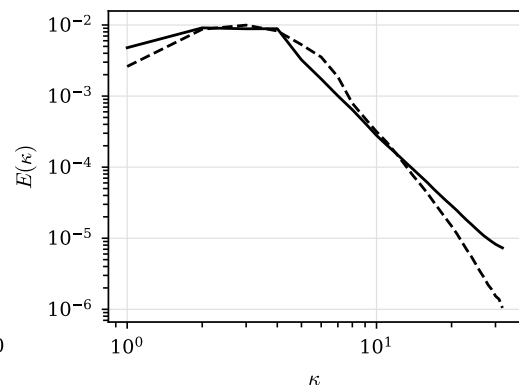

Latent-step consistency

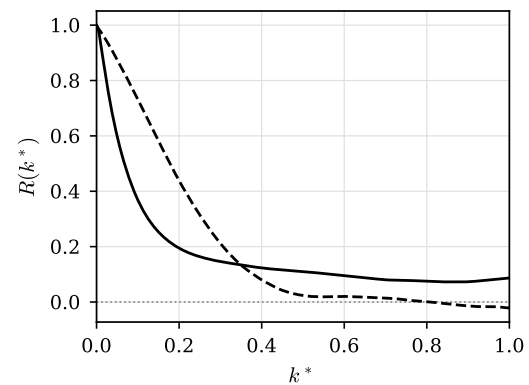

Increased capacity

