



NM-SCRC-I (EB) validity — PAC histogram over 100 calibration draws ($\Delta = 0.05$)

1B probe

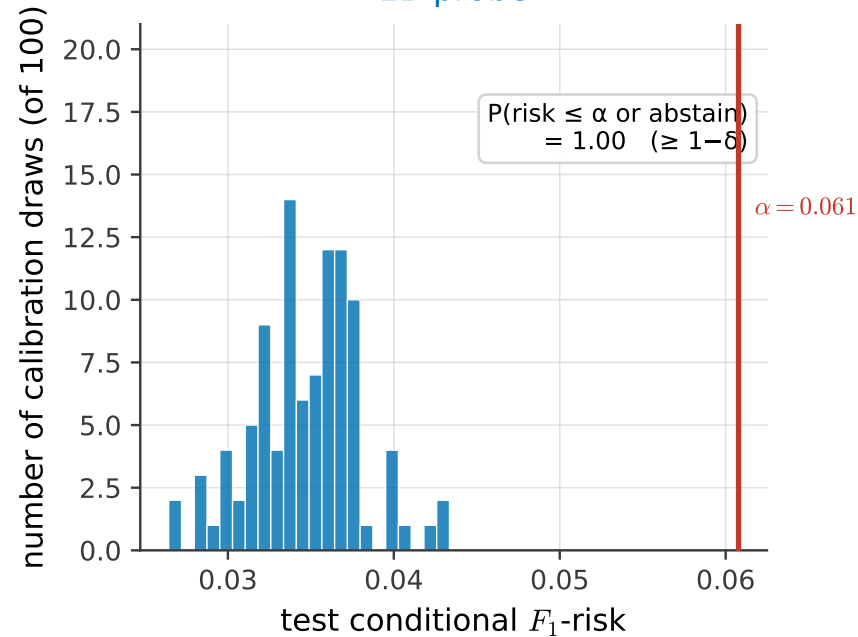

3B probe

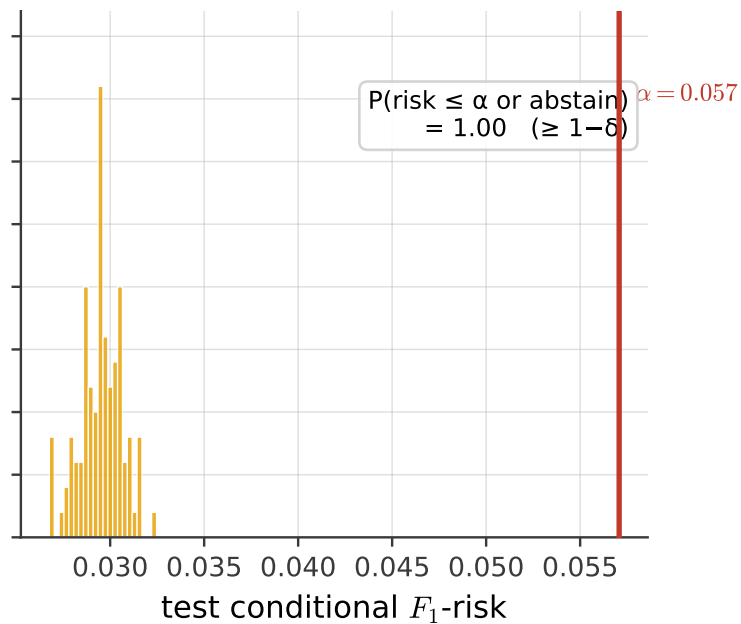

8B probe

