

Harmony: Dye-VL -ClearLift - Chart

For MedSpa/Provider Use Only — Not for Patient Completion.



Patient Name _____

DOB: _____

Date of Procedure ____/____/20__

Supervising Physician: ☐ Allie Angel MD MHA ☐ Sergio Angel MD MHA

Assistant ☐ Elisa Cavallin ☐ Jennifer Romero


Fitzpatrick Skin Type: ☐ I ☐ II ☐ III ☐ IV ☐ V ☐ VI Medical History Completed ☐ Yes ☐ No Consent Signed ☐ Yes ☐ No

Wavelength Specific Eyewear: ☐ Patient ☐ Staff Smoke Evacuator used: ☐ Yes ☐ No

Procedure: ☐ Alma harmony: Dye-VL ☐ Harmony -ClearLift ☐ Harmony

Area treated: _____

Image chart.

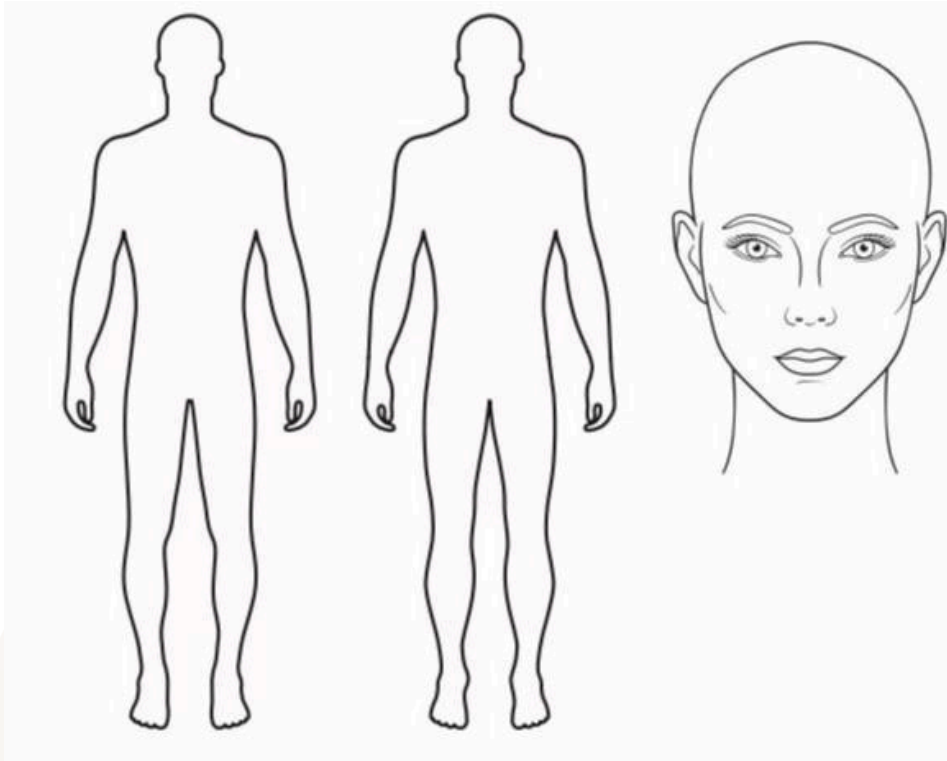

DyeVL/SHR:

Fluence: _____ Pulse Width: _____ Total Energy/kJ's: _____

% Cooling: _____

Q-Switch YAG:

ClearLift: Fluence: _____ PRR/Hz: _____ Accumulative Energy (J): _____

Stacks: _____ Passes: _____ Tips: -2 -1 0 +1 +2

CVD/532nm tip: Spot Size: _____ Energy (mJ): _____ Hz: _____

kiwi MEDSPA

MEDICAL WEIGHT LOSS & AESTHETICS




Was the test patch performed? ☐ Yes ☐ No


Result: _____

Skin reaction at end of procedure Note any skin reaction discernible at end of procedure,
i.e. edema, erythema, etc:



SOAP NOTES	
Subjective	
Objective	
Assessment	
Plan	

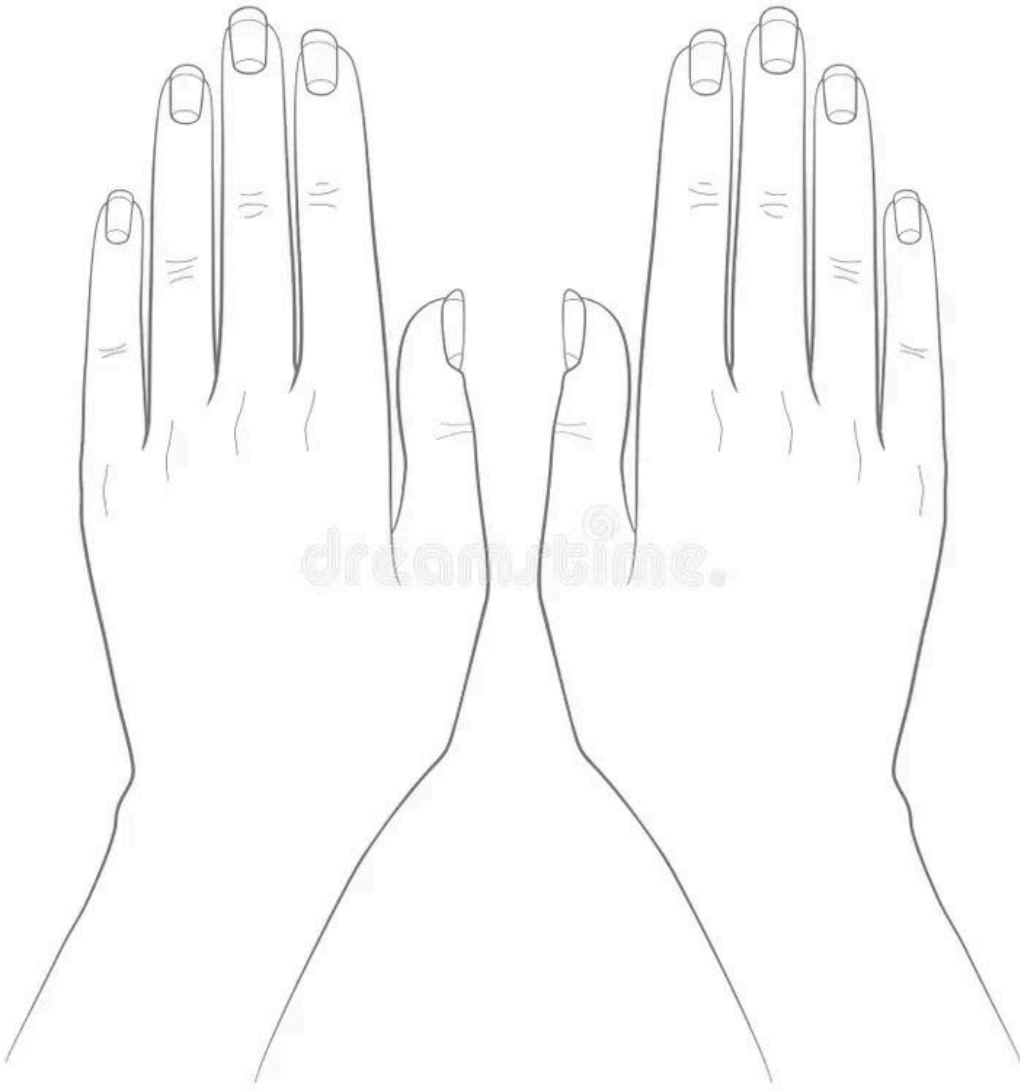

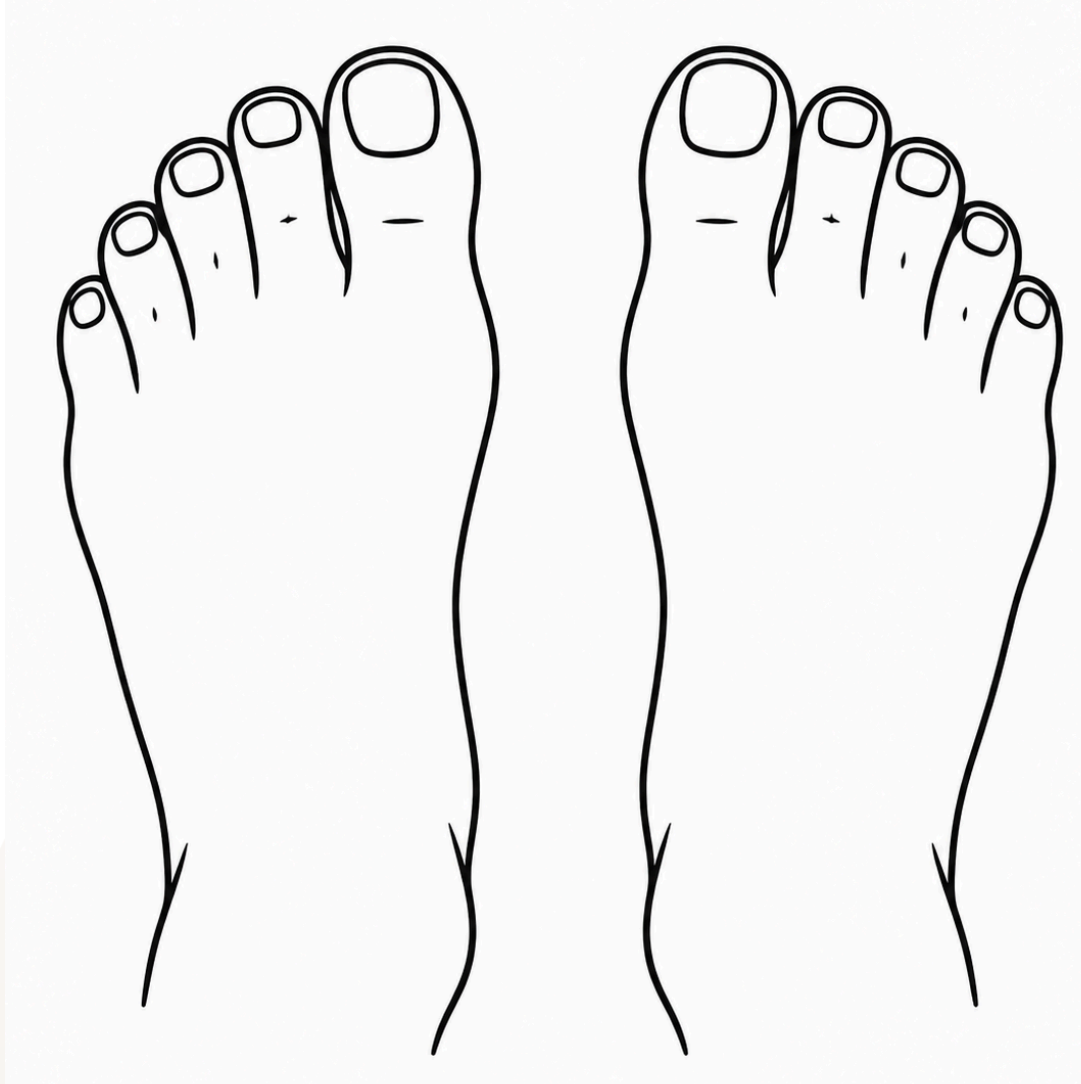

Photos / Medical Record ☐ Pre-treatment photos taken for clinical record ☐ Post-treatment photos taken for clinical record

- ☐ Patient tolerated procedure.
- ☐ Post-procedure instructions given to the patient.
- ☐ Follow-up instructions given to the patient.

Physician signature *

☐ I confirm that this signature is legally binding.