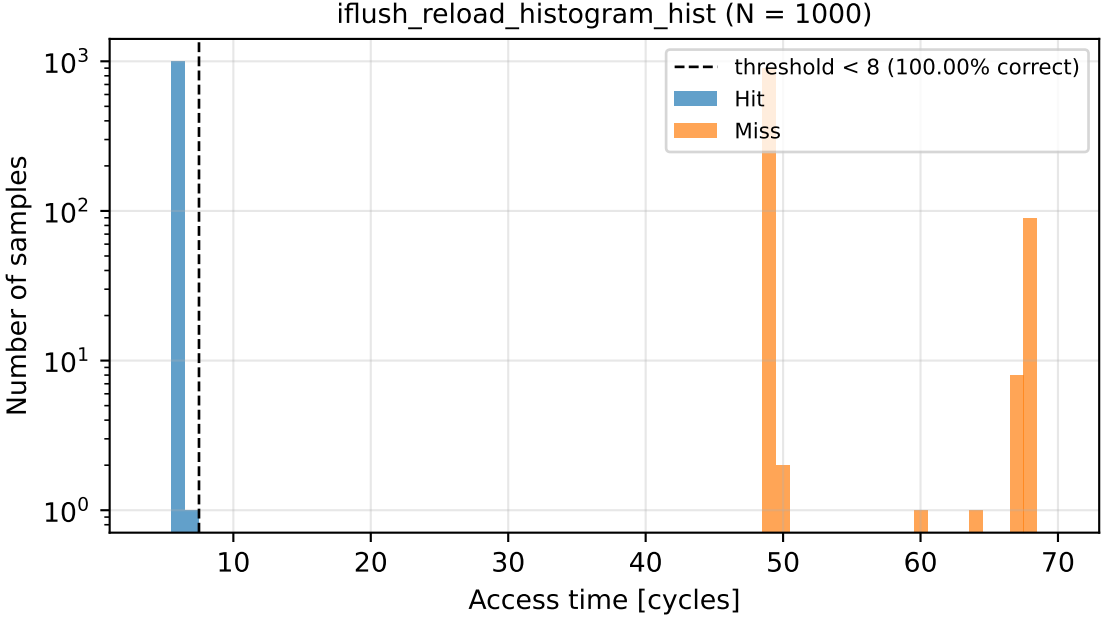
iflush_reload_histogram_hist (N = 1000)
threshold < 8 (100.00% correct)
Hit
Miss
Number of samples
10^3
10^2
10^1
10^0
10
20
30
40
50
60
70
Access time [cycles]