


Eigenvalue-weighted coefficient: held-out exact-null calibration under GTR PF06346

Exact-null held-out target rejection with 95% Wilson intervals

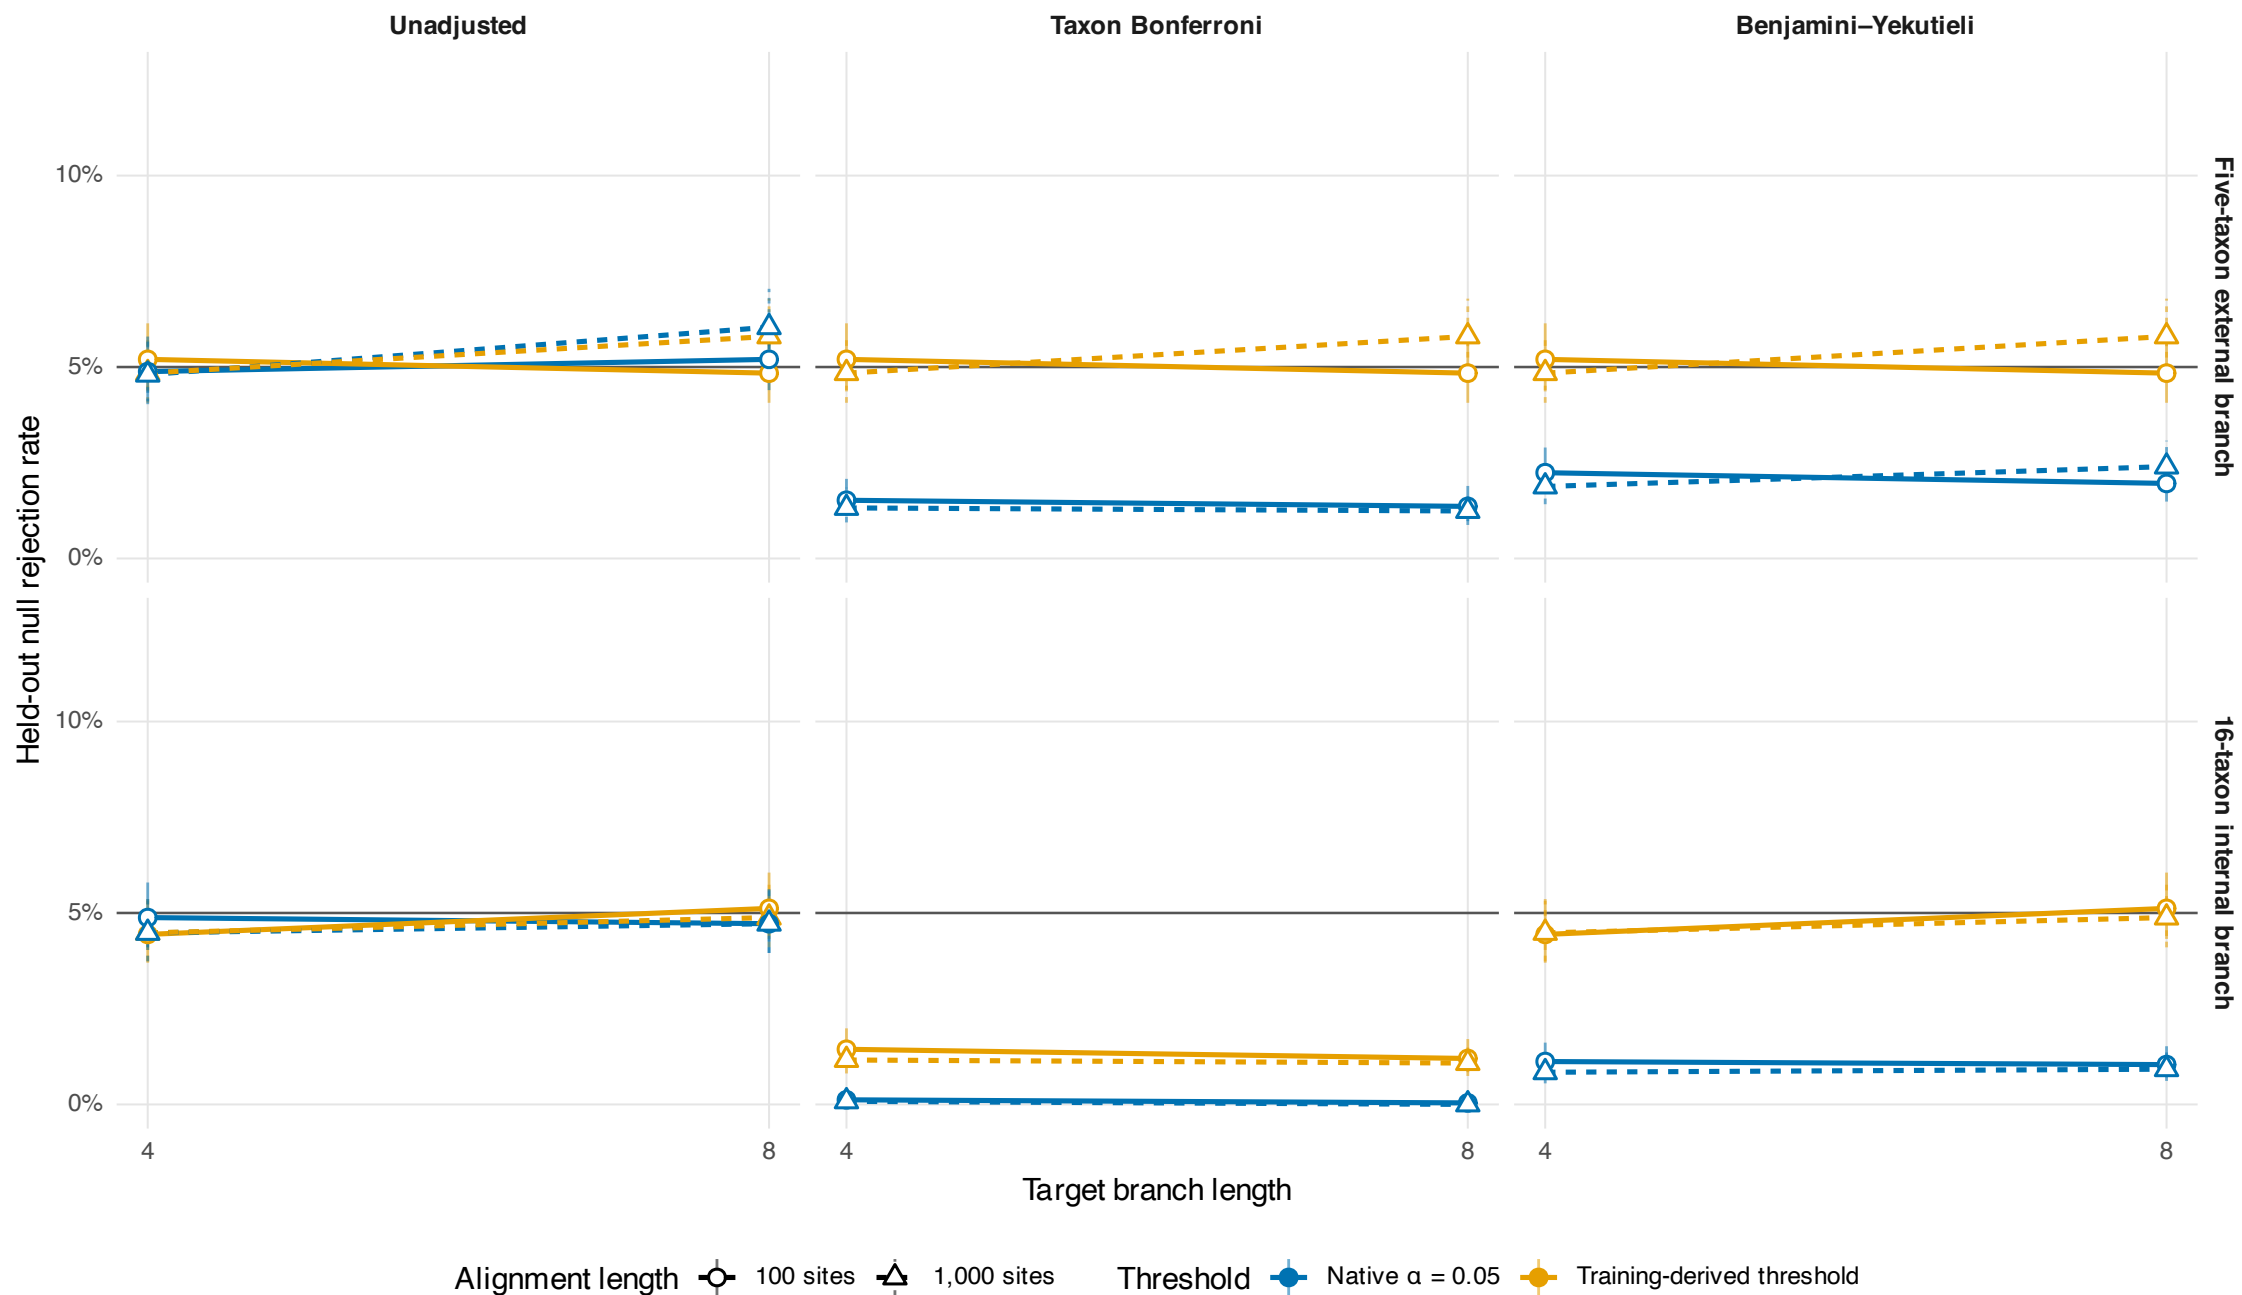

The training-derived threshold is estimated from 2,500 independent training replicates and evaluated on 2,500 held-out replicates.