

RD III4-R

110413391

A	PA%	PA Corr	PA % Corr

110413392

FIGURE 2
MONITORING OF RESPIRATORY FUNCTION IN CONSCIOUS ANIMALS.
SHOWING TWO RESPIRERS, FRODO'S TO NOSE, MINE AND
BODY PLETHYSMOGRAPH MONITORING DEVICES



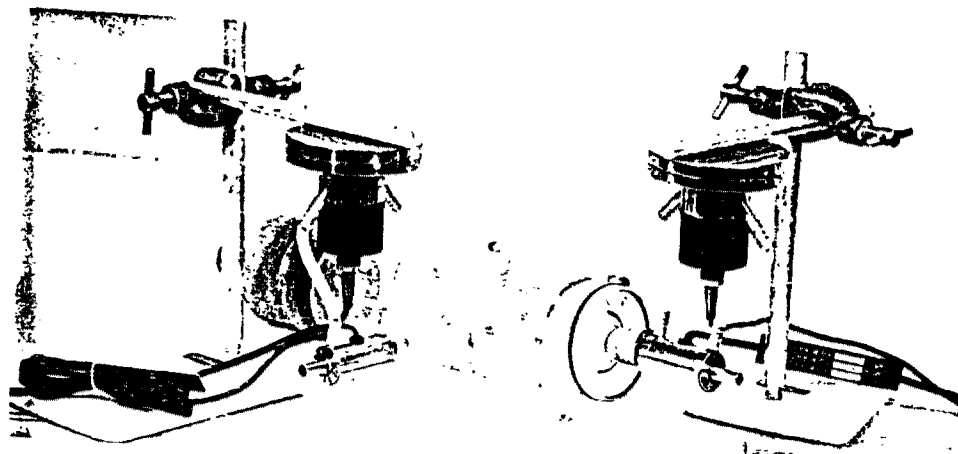


FIGURE 3
PART OF SMOKE EXPOSURE SYSTEM, SHOWING BODY PLETHYSMOGRAPHS
ATTACHED TO SMALL EXPOSURE CHAMBER

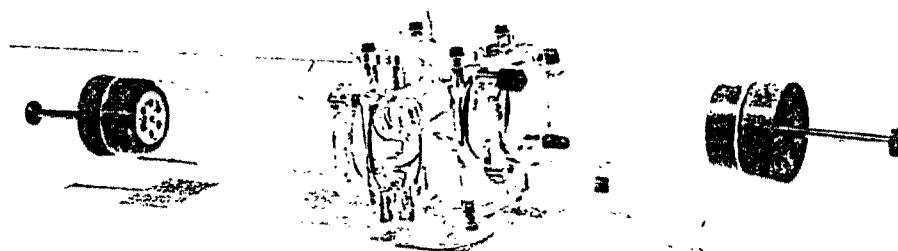

110413393


APR 1955
GENERAL ELECTRIC COMPANY
RESEARCH AND DEVELOPMENT
DIVISION
Schenectady, New York

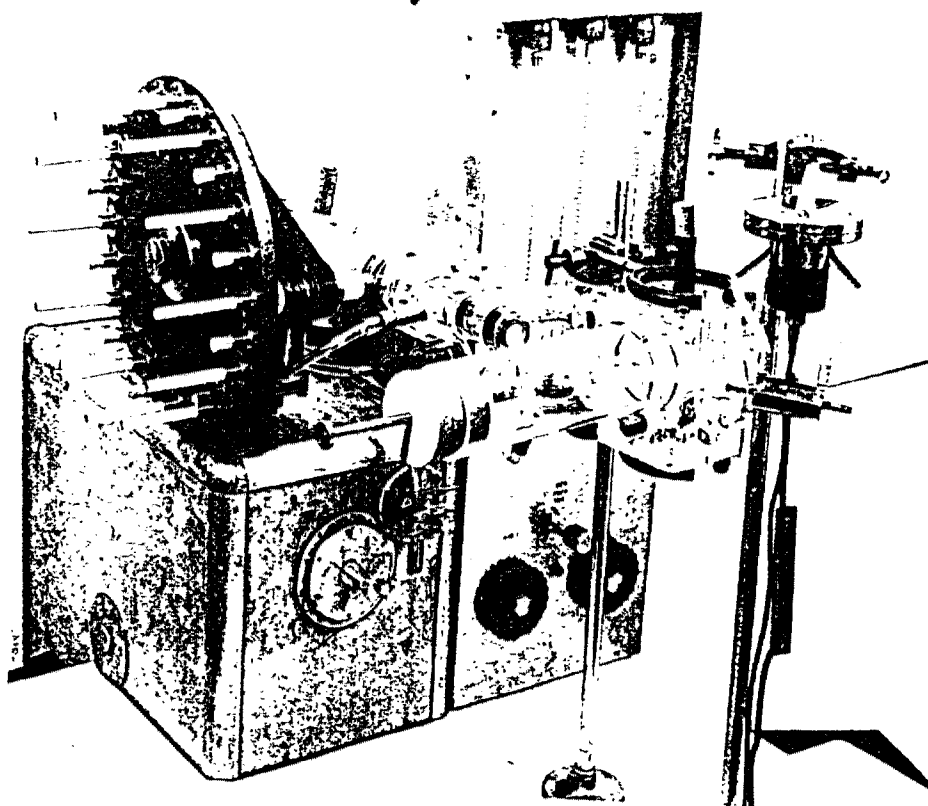


11041339

FIGURE 12a & b

EXAMPLES OF RESPIRATION PATTERNS IN a) RAT AND b) CHINA PIC.
 S.A.T. IS 2-4 SECONDS OF STIMULATION. THE 3-4 SECONDS INTERVALS
 TO STIMULATION BEING INTO THE NEXT SECONDS.
 (APPROXIMATELY 10 SECS) L.F. 1000 Hz

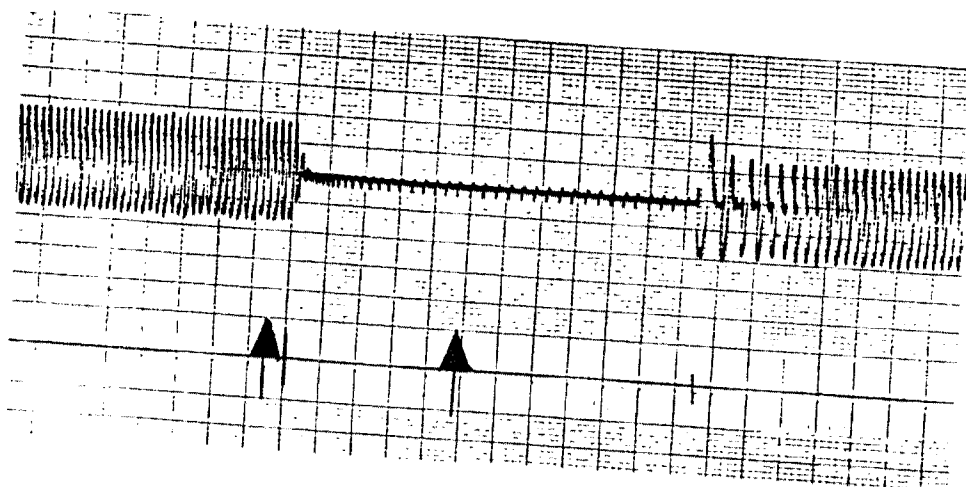

(a) RAT

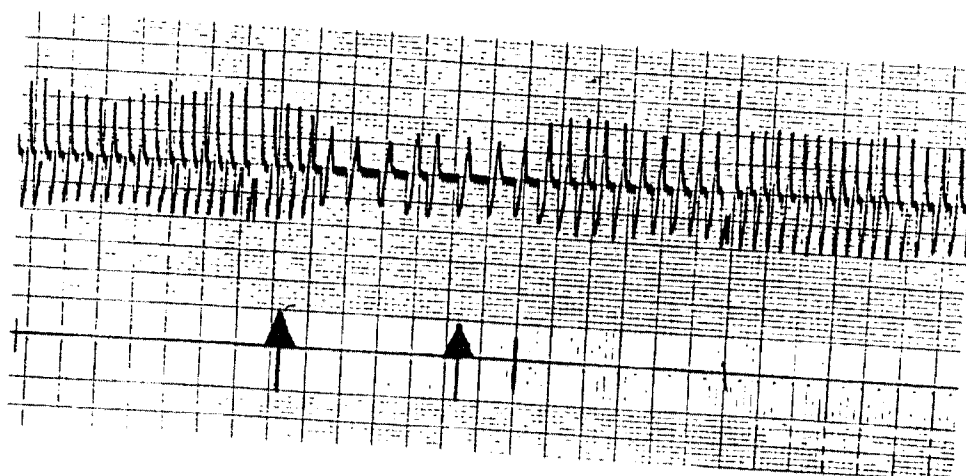

(b) CHINA PIC

11041359