

YOSEMITECH

NH4_N Sensor

MODBUS RTU
Programmer Manual

Table of Contents

1	MODBUS RTU Overview	3
1.1	Scope	3
1.2	MODBUS Command Structure	3
1.3	MODBUS RTU for YOSEMITECH's NH4_N Sensor	5
1.4	MODBUS RTU Function Code for YOSEMITECH's NH4_N Sensor	5
1.5	Data formats in NH4_N sensor.....	7
2	MODBUS RTU Commands for NH4_N Sensor.....	10
2.1	Overview.....	10
2.2	Command Description	10
3	Procedure to get NH4_N value	21

1 MODBUS RTU Overview

1.1 Scope

This document is about MODBUS of Self-cleaning NH₄_N probes with hardware Rev1.0 and software Rev1.6 or later. This document is intended for software programmers with detailed information about MODBUS RTU protocols.

1.2 MODBUS Command Structure

Data format in this document:

- Binary number – shown with suffix B. For example: 10001B
- Decimal number – without nay suffix. For example: 256
- Hexadecimal number—shown with prefix 0x. For example: 0x2A
- ASCII character or string – shown with quotation marks. For example: "YL1014010022"

1.2.1 Command Structure

MODBUS defines a simple protocol data unit (PDU), which is transparent to communication layer.

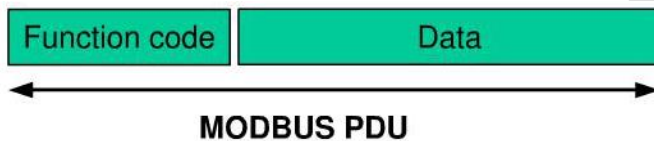


Figure 1: MODBUS Protocol Data Unit

The mapping of MODBUS protocol on a specific bus or network introduces some additional fields on the Protocol Data Unit. The client that initiates a MODBUS transaction builds the MODBUS PDU, and then adds fields in order to build the appropriate communication PDU.

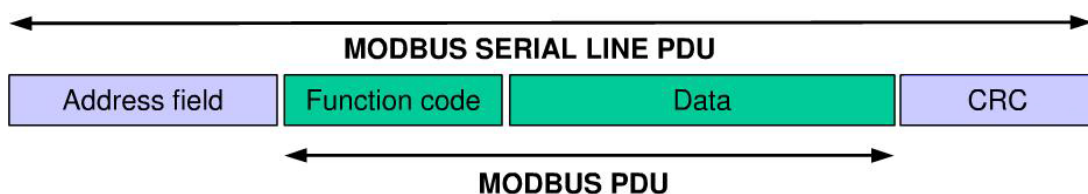


Figure 2: MODBUS Structure for Serial Communication

On a MODBUS serial bus, address field only includes addresses for slave devices.

Note:

- Slave address range for NH₄_N sensor is: 1...247
- Master device sends a "request frame" with a targeted slave address. When slave device responses, it has to put its own address in the "response frame", so that master device knows where the response comes from.
- Function code indicates type of operations

- CRC is the result of redundancy check.

1.2.2 MODBUS RTU Transmission Mode

When devices communicate on a MODBUS using RTU (remote terminal unit) mode, each 8-bit byte message contains two 4-bit hexadecimal characters. The main advantage of the RTU mode is that it has higher character density, which enables better throughput compare to ASCII mode at same baud rate. Each RTU message must be transmitted in a continuous string of characters.

RTU mode format for each byte (11 bits):

Encoding system	8 bit binary
	Each 8-bit packet contains 4-bit hexadecimal characters (0-9, A-F)
Bit per byte:	1 start bit
	8 data bits, least significant bit first
	No parity check
	1 stop bits
Baud rate:	9600bps

Serial transmission of characters:

Every character or byte is sent under this sequence (left to right):

Least Significant Bit (LSB).....Most Significant Bit(MSB)

Start	1	2	3	4	5	6	7	8	Stop
-------	---	---	---	---	---	---	---	---	------

Figure 3: RTU Mode Bit Sequence

CRC Field Structure:

Redundancy check (CRC16)

Frame Structure:

Slave address	Function Code	Data	CRC	
1 byte	1 byte	0...252 bytes	2 bytes	
			CRC Low	CRC High

Figure 4: RTU Message Frame Structure

Maximum size of MODBUS frame is 256 bytes.

1.2.3 MODBUS RTU Message Frame

In RTU mode, message frames need to be separated by an idle interval of at least 3.5 character lengths. In rest of this document, this idle interval is called t3.5.

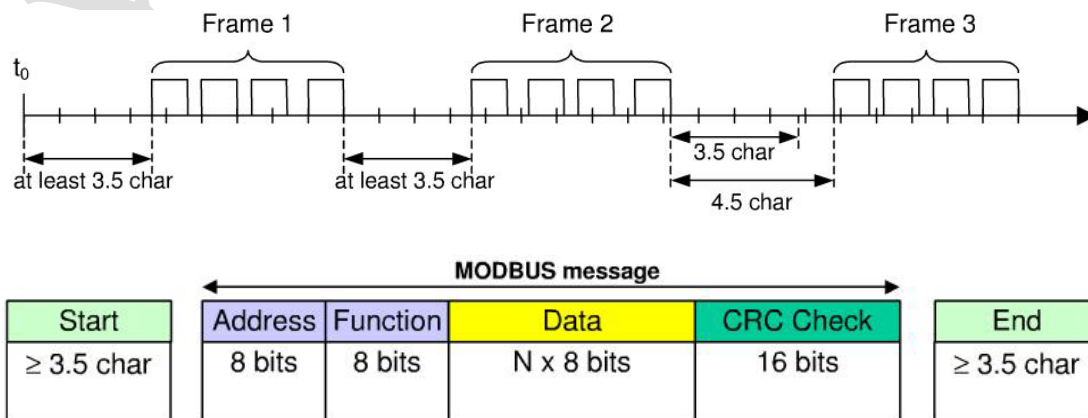


Figure 5: RTU Message Frame

Entire message frame must be sent as continuous stream of characters.

If idle time between two characters is longer than 1.5 characters, the message frame will be considered incomplete, and will be discarded by receiving side.

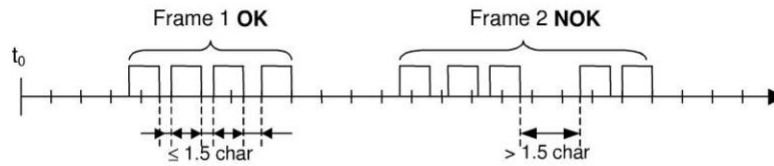


Figure 6: Frame transmission

1.2.4 MODBUS RTU CRC Check

In RTU mode, the error checking field is based on a cyclical redundant checking (CRC) method. The CRC field checks entire content of MODBUS message, regardless of the existence of parity check bit. CRC16 checking method is utilized. CRC result is a 16-bit value with two 8-bit bytes, low order 8-bit byte first followed by high order 8-bit byte.

1.3 MODBUS RTU for YOSEMITECH's NH4_N Sensor

Based on standard MODBUS definition, message frame starts with t3.5 idle interval, and similarly, ends with t3.5 idle interval. Device address and Function code are both 8-bit byte. Data character string has n*8 bits, it contains information about register start/end address and number of registers for read/write operation. CRC field is 16 bit in length.

	Start	Device address	Function code	Data	CRC		End
Value	Idle for 3.5 character length	1-247	Comply with MODBUS function code format	Comply with MODBUS data format	CRC Low	CRC High	Idle for 3.5 character length
Length (byte)	3.5	1	1	n	1	1	3.5

Figure 7: Message frame structure for Yosemitech's MODBUS

1.4 MODBUS RTU Function Code for YOSEMITECH's NH4_N Sensor

YOSEMITECH's NH4_N sensor has two MODBUS function codes:

0x03: Read registers 0x10: Write registers

1.4.1 MODBUS Function Code 0x03: Read Registers

This function code is to read a block of continuous registers from a remote device. Request PDU defines start address and number of registers for the read operation. Register addressing starts from 0. Therefore, addresses for register 1-16 are 0-15. Data for each register in Response

message have two bytes. For each register data, first byte is for high bits, and second byte for low bits.

Request Frame:

Function code	1 Byte	0x03
Start address	2 Bytes	0x0000....0xffff
Number of registers	2 Bytes	1...125

Figure 8: Request frame for read registers

Response Frame:

Function code	1 byte	0x03
Number of byte	1 byte	$N \times 2$
Register data	$N \times 2$ bytes	

N = number of registers

Figure 9: Response frame for read registers

Below is an example of Request and Response frames (Read register 108-110. Register 108 is read only with 2-byte value of 0X022B. Registers 109-110 have values of 0X0000 and 0X0064).

Request Frame		Response Frame	
Data format	Hexadecimal	Data Format	Hexadecimal
Function code	0x03	Function code	0x03
Start address(high bits)	0x00	Number of bytes	0x06
Start address (low bits)	0x6B	Register value (high bits, 108)	0x02
Number of registers (high bits)	0x00	Register value (low bits, 108)	0x2B
Number of registers (low bits)	0x03	Register value (high bits, 109)	0x00
		Register value (low bits, 109)	0x00
		Register value (high bits, 110)	0x00
		Register value (low bits, 110)	0x64

Figure 10: Example of request frame and response frame for read operation

1.4.2 MODBUS Function Code 0x10: Write Registers

This function code is to write a block of continuous registers at a remote device. Request frame contains register data. Each register data have two character bytes. Response frame contains function code, start address, and number of registers that completed write operation.

Request Frame:

Function code	1 byte	0x10
Start address	2 bytes	0x0000....0xffff
Number of registers	2 bytes	0x0001....0x0078
Number of bytes	1 byte	$N \times 2$
Register data	$N \times 2$ bytes	value

N = number of registers

Figure 11: Request frame for write operation

Response Frame:

Function Code	1 byte	0x10
Start address	2 bytes	0x0000....0xffff
Number of registers	2 bytes	1...123(0x7B)

N = number of registers

Figure 12: Response frame for write operation

Below is an example of Request Frame and Response frame (write 0x000A and 0x0102 to two registers starting from address 2):

Request Frame		Response Frame	
Data Format	Hexadecimal	Data Format	Hexadecimal
Function code	0x10	Function code	0x10
Start address (high bits)	0x00	Start address (high bits)	0x00
Start address (low bits)	0x01	Start address (low bits)	0x01
Number of registers (high bits)	0x00	Number of registers (high bits)	0x00
Number of registers (low bits)	0x02	Number of registers (low bits)	0x02
Number of bytes	0x04		
Register value (high bits)	0x00		
Register value (low bits)	0x0A		
Register value (high bits)	0x01		
Register value (low bits)	0x02		

Figure 13: Example of Request frame and response frame for write operation

1.5 Data formats in NH4_N sensor

1.5.1 Floating-point number

Definition: floating point number, comply with IEEE754 (single precision)

Note	Sign	Exponent	Fraction	Total
bit	31	30...23	22...0	32
Exponent deviation	127			

Figure 14: Single floating point number definition (4 bytes, 2 MODBUS registers)

Example: Convert decimal number 17.625 to binary number

Step 1: Convert decimal number 17.625 to a floating point number with binary format

First, convert integer to binary

$$17_{\text{decimal}} = 16 + 1 = 1 \times 2^4 + 0 \times 2^3 + 0 \times 2^2 + 0 \times 2^1 + 1 \times 2^0$$

Thus, integer 17 in binary format is 10001B

Then convert decimal part to binary

$$0.625_{\text{decimal}} = 0.5 + 0.125 = 1 \times 2^{-1} + 0 \times 2^{-2} + 1 \times 2^{-3}$$

Thus, 0.625 in binary format is 0.101B

Combine above together, 17.625 in binary format is 10001.010B

Step 2: Calculate exponent

Left shift the binary number 10001.010B until only bit left before the decimal point ---
 $10001.010B = 1.0001101B \times 2^4$, so exponent value is 4. By adding 127, we have 131, which
 is 10000011B in binary format

Step 3: Get fraction

Fraction is simply the number after decimal point. Thus from 1.0001101B, fraction number is 0001101B. IMPORTANT NOTE about the 23 bit fraction number: the first bit which on the left side of decimal point is hidden bit and does not need to be compiled.

Step 4: Sign definition

Sign bit is 0 if the number is positive. Sign is 1 if the number is negative. For 17.625, sign 17.625, sign bit is 0.

Step 5: Convert to floating point number

1 Sign bit	+	8-bit exponent	+	23-bit fraction
0		10000011		00011010000000000000000B

(Corresponding hexadecimal number is 0x418D0000)

Sample code:

1. If your compiler has similar library functions, it can be called directly. For example if C language is used, we can directly call memcpy() function in C library to convert floating point number. Sample code:

```
float    floatdata;//floating point data to be converted
void*    outdata;
memcpy(outdata,&floatdata,4);
```

If floatdata=17.625,

In little-endian storage mode after the function is called:

Value at address of outdata is 0x00
 Value at address of (outdata+1) is 0x00
 Value at address of (outdata+2) is 0x8D
 Value at address of (outdata+3) is 0x41

In big-endian storage mode after the function is called:

Value at address of outdata is 0x41
 Value at address of (outdata+1) is 0x8D
 Value at address of (outdata+2) is 0x00
 Value at address of (outdata+3) is 0x00

2. If your compiler doesn't have the conversion function, then the following function can be used:

```
void memcpy(void *dest,void *src,int n)
{
    char *pd = (char *)dest;
    char *ps = (char *)src;
    for(int i=0;i<n;i++)    *pd++ = *ps++;
}
```

Then you can get same result by calling this function memcpy(outdata,&floatdata,4);

Example: Convert binary floating point number 0100 0010 0111 1011 0110 0110 0110 0110B to a decimal number

- Step 1: Separate this binary number 0100 0010 0111 1011 0110 0110 0110 0110B and get values of Sign, exponent and fraction.

0	10000100	11110110110011001100110B
1 Sign bit	8-bit exponent	23-bit fraction

Sign bit(s): 0

$$\begin{aligned}\text{Exponent(E): } 10000100\text{B} &= 1 \times 2^7 + 0 \times 2^6 + 0 \times 2^5 + 0 \times 2^4 + 0 \times 2^3 + 1 \times 2^2 + 0 \times 2^1 + 0 \times 2^0 \\ &= 128 + 0 + 0 + 0 + 0 + 4 + 0 + 0 = 132\end{aligned}$$

$$\text{Fraction(M): } 11110110110011001100110\text{B} = 8087142$$

Step 2: Calculate decimal value

$$\begin{aligned}D &= (-1)^S \times (1.0 + M/2^{23}) \times 2^{E-127} \\ &= (-1)^0 \times (1.0 + 8087142/2^{23}) \times 2^{132-127} \\ &= 1 \times 1.964062452316284 \times 32 \\ &= 62.85\end{aligned}$$

Reference code:

```
float floatTODecimal(long int byte0, long int byte1, long int byte2, long int byte3)
{
    long int realbyte0, realbyte1, realbyte2, realbyte3;
    char S;
    long int    E, M;
    float D;
    realbyte0 = byte3;
    realbyte1 = byte2;
    realbyte2 = byte1;
    realbyte3 = byte0;

    if((realbyte0 & 0x80) == 0)
    {
        S = 0; //Positive
    }
    else
    {
        S = 1; //Negative
    }
    E = ((realbyte0 << 1) | (realbyte1 & 0x80) >> 7) - 127;
    M = ((realbyte1 & 0x7f) << 16) | (realbyte2 << 8) | realbyte3;
    D = pow(-1, S) * (1.0 + M / pow(2, 23)) * pow(2, E);
    return D;
}
```

Note:

- Function parameters byte0, byte1, byte2 and byte3 represent the 4 sections of a binary floating number.
- Return value is value of decimal number after conversion

For example when a command is sent to a sensor to get temperature value, response frame from the sensor will have measured temperature. If the values are 4 byte floating point number 0x00, 0x00, 0x8d, 0x41, then the following function can be used to get temperature in decimal value:

```
float temperature = floatTODecimal( 0x00, 0x00, 0x8d, 0x41);
```

and temperature = 17.625.

1.5.2 Characters

Definition: Character is shown by ASCII code.

Example: String “YL” could be shown by corresponding ASCII codes (refer to ASCII character chart)

“Y” is 0x59

“L” is 0x4C

2 MODBUS RTU Commands for NH4_N Sensor

2.1 Overview

In order to communicate with NH4_N probe via MODBUS RTU, master terminal software will be needed. MODBUS RTU is an open standard. There are free commercial software tools available. For applications described in this document, MODBUS register address starts from 1. However, slave address in MODBUS protocol starts from 0, and usually master software compiles addresses. For example, register address 2090 will be compiled by master software as address 2089.

2.2 Command Description

2.2.1 Set Slave Device ID

Purpose: Set MODBUS slave address to a sensor probe. Range of address is 1~247.

Sensor probe slave address can be set via MODBUS register 0x3000:

Start address	Number of registers	Register 1	MODBUS Function code
0x3000	0x01	New Slave address	0x10

Figure 15: Register definition of Set Slave ID Command

Below is an example of request and response frames for setting slave device ID command. Old slave address is 0x01, new address is 0x14.

Definition	Address	Function code	Start address		Number of registers		Number of byte	Register value		CRC	
Byte	0	1	2	3	4	5	6	7	8	9	10
Value	0x01	0x10	0x30	0x00	0x00	0x01	0x02	0x14	0x00	0x99	0x53

Figure 16: Request frame to Set Slave ID

*Note: byte 8 is reserved

Definition	Address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x10	0x30	0x00	0x00	0x01	0x0E	0xC9

Figure 17: Response frame for Set Slave ID Command

2.2.2 Get SN

Purpose: Get sensor probe's serial number (SN). Each sensor probe has a unique SN.

Serial Number can be read from 7 continuous MODBUS registers starting from address 0x0900.

Start Address	Number of registers	Register 1-7	MODBUS Function code
0x0900	0x07	SN	0x03

Figure 18: Register definition of Get SN Command

Below is an example of request and response frames to get SN "YL1014010022" from a slave device (address 0x01).

Definition	Address	Function code	Starting address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x09	0x00	0x00	0x07	0x07	0x94

Figure 19: Request frame to Get SN Command

Definition	Address	Function code	Number of byte	Register value			CRC	
Byte	0	1	2	3	4-15	16	17	18
Value	0x01	0x03	0x0E	0x00	"YL1014010022"	0x00	0x4c	0x5f

Figure 20: Response frame for Get SN Command

Note: SN value is in ASCII code as below:

Byte	4	5	6	7	8	9	10	11	12	13	14	15
Value	0x59	0x4C	0x31	0x30	0x31	0x34	0x30	0x31	0x30	0x30	0x32	0x32

Figure 21: Sensor probe's SN

2.2.3 Get pH and potential Value (ORP)

Purpose: Get current pH and potential value (ORP), the unit is mV.

The pH and potential value can be read from 4 continuous MODBUS registers starting from address 0x2600.

Start address	Number of registers	Register 1-2	Register 3-4	MODBUS 功能码
0x2600	0x04	potential value	pH value	0x03

Figure 25: Request frame to Get pH and potential value(ORP) Command

Below is an example of request and response frames for getting pH and potential value command, assuming slave device address is 0x01, returned pH value is 7 and potential value (ORP) is -6.56mV.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x26	0x00	0x00	0x04	0x4F	0x41

Figure 26: Request frame to Get pH and potential value (ORP) Command

Definition	Device address	Function code	Number of bytes	Register value			CRC	
------------	----------------	---------------	-----------------	----------------	--	--	-----	--

Byte	0	1	2	3~6	7~10	11	12
Value	0x01	0x03	0x08	-6.56	7	0x5C	0xE6

Figure 27: Response frame for Get pH and potential value (ORP) Command

potential value (3-6)				pH value (7-10)			
0x85	0xEB	0xD1	0xC0	0x00	0x00	0xE0	0x40

Figure 28: Registers definition for pH and potential value (ORP).

2.2.4 Get NH4+ and K+ in mV

Purpose: Get current NH4+ and K+, the unit is mV.

The NH4+ and K+ can be read from 4 continuous MODBUS registers starting from address 0x3700.(For now being, K+ value is ignored)

Start address	Number of registers	Register 1-2	Register 3-4	MODBUS 功能码
0x3700	0x04	NH4+	K+	0x03

Figure 29: Request frame to Get NH4+ and K+ Command

Below is an example of request and response frames for getting NH4+ and K+ command, assuming slave device address is 0x01, returned NH4+ value is -20.1 and K+ is -32.2mV.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x37	0x00	0x00	0x04	0x4A	0x7D

Figure 30: Request frame to Get NH4+ and K+ Command

Definition	Device address	Function code	Number of bytes	Register value		CRC	
Byte	0	1	2	3~6	7~10	11	12
Value	0x01	0x03	0x08	-20.1	-32.2	0x5B	0x61

Figure 31: Response frame for Get NH4+ and K+ Command

NH4+ value (3-6)				K+value (7-10)			
0xCD	0xCC	0xA0	0xC1	0xCD	0xCC	0x00	0xC2

Figure 32: Registers definition for NH4+ and K+.

2.2.5 Get NH3_N NH4+ and K+ in mg/L

Purpose: Get NH3_N NH4+ and K+ value after temperature compensation, the unit is mg/L.

The NH3_N ,NH4+ and K+ can be read from 6 continuous MODBUS registers starting from address 0x2800.

Start address	Number of registers	Register 1-2	Register 3-4	Register 5-6	MODBUS 功能码
0x2800	0x06	NH3_N	K+	NH4+	0x03

Figure 33: Request frame to Get NH3_N ,NH4+ and K+ Command

Below is an example of request and response frames for getting NH3_N ,NH4+ and K+ command, assuming slave device address is 0x01, returned NH3_N value is 7.6,NH4+ value is 5.2 and K+ is 1.0 mg/L.

Definition	Device	Function	Start address	Number of	CRC
------------	--------	----------	---------------	-----------	-----

	address	code			registers			
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x28	0x00	0x00	0x06	0xCC	0x68

Figure 34: Request frame to Get NH3_N ,NH4+ and K+ Command

Definition	Device address	Function code	Number of bytes	Register value			CRC	
Byte	0	1	2	3~6	7~10	11~14	15	16
Value	0x01	0x03	0x0C	7.6	1.0	5.2	0x6C	0x7D

Figure 35: Response frame for Get NH3_N ,NH4+ and K+ Command

NH4_N value (3~6)				K+ value (7~10)				NH4+ value(11~14)			
0x33	0x33	0xF3	0x40	0x00	0x00	0x80	0x3F	0x66	0x66	0xA6	0x40

Figure 36: Registers definition for NH3_N ,NH4+ and K+.

2.2.6 Get temperature value

Purpose: Get current temperature value , the unit is C.

Temperature can be read from 2 continuous MODBUS registers starting from address 0x2400.

Start address	Number of registers	Register 1-2	MODBUS function code
0x2400	0x02	temperature value	0x03

Figure 37: Request frame to Get temperature Command

Below is an example of request and response frames for getting temperature command, assuming slave device address is 0x01, returned temperature value is 15.8.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x24	0x00	0x00	0x02	0xCE	0xFB

Figure38: Request frame to Get temperature Command

Definition	Device address	Function code	Number of bytes	Register value	CRC	
Byte	0	1	2	3-6	11	12
Value	0x01	0x03	0x04	15.8	0xE4	0x50

Figure 39: Response frame for Get temperature Command

Temperature value (3~6)			
0xCD	0xCC	0x7C	0x41

Figure 40: Registers definition for temperature.

2.2.7 Get Software and Hardware Rev

Purpose: Get current hardware and software Release Version

Hardware and software release version numbers of a sensor probe can be read from 2 continuous registers starting from address 0x0700.

Start address	Number registers	Register 1	Register 2	MODBUS function code
0x0700	0x02	HW Rev	SW Rev	0x03

Figure 41: Register definition for Get Software and Hardware Rev Command

Below is an example of request and response frames for getting hardware and software release version, assuming device slave address is 0x01, returned value for hardware Rev is 1.0 and software rev is 1.0.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x07	0x00	0x00	0x02	0xc5	0x7f

Figure 42: Request frame to Get Hardware and Software Rev Command

Definition	Device address	Function code	Number of bytes	Register value				CRC	
Byte	0	1	2	3-4		5-6		7	8
Value	0x01	0x03	0x04	0x01	0x00	0x01	0x00	0xfa	0x5f

Figure 43: Response frame for Get Hardware and Software Rev Command

2.2.8 Stop Measurement

Purpose: After stable test results is obtained, stop measurement activities.

MODBUS register 0x2E00 is used for this command.

Start address	Number of registers	MODBUS function code
0x2E00	0x01	0x03

Figure 44: Register definition of Stop Measurement Command

Below is an example of request and response frames for a device with slave address 0x01 to stop measurement activities.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x2E	0x00	0x00	0x01	0x8D	0x22

Figure 45: Request frame to Stop Measurement Command

Definition	Device address	Function code	Number of bytes	Register value	CRC	
Byte	0	1	2	3~4	5	6
Value	0x01	0x03	0x00	meaningless		

Figure 46: Response frame for Stop Measurement Command

2.2.9 Set pH Electrode Coefficients

Purpose: Recover pH factory calibration coefficients K1~K6. **K1=6.86, K2=-6.72, K3=0.04, K4=6.86, K5=-6.56, K6=-1.04** by default.

Customer coefficients can be set at 12 continuous MODBUS registers starting from address 0x2900.

Start address	Number of registers	Register 1-12	MODBUS function code
0x2900	0x0C	K1~K6	0x10

Figure 47: Register definition of Set pH Customer Calibration Coefficients Command

Below is an example of request and response frames for setting customer calibration coefficients, assuming slave address is 0x01.

Definition	Device address	Function code	Start address		Number of registers		Number of bytes	Register value	CRC	
Byte	0	1	2	3	4	5	6	7-30	15	16
Value	0x01	0x10	0x29	0x00	0x00	0x0C	0x18	K1~K6	0x94	0x59

Figure 48: Request frame to Set pH Customer Calibration Coefficients Command

Note: Coefficients K1~K6, floating point numbers in little-endian storage mode

K1(7~10)				K2(11~14)				K3(15~18)				K4(19~22)			
0x1f	0x85	0xdb	0x40	0x3d	0x0a	0xd7	0xc0	0x0a	0xd7	0x23	0x3d	0x1f	0x85	0xdb	0x40
K5(23~26)				K6(27~30)											
0x85	0xeb	0xd1	0xc0	0xb8	0x1e	0x85	0xbf								

Figure 49: Registers for coefficients K1~K6

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x10	0x29	0x00	0x00	0x0C	0xC8	0x50

Figure 50: Response frame for Set pH Customer Calibration Coefficients Command

2.2.10 Get pH Electrode Coefficients

Purpose: Get pH Customer Calibration Coefficients .

The Customer Calibration Coefficients can be read from 12 continuous MODBUS registers starting from address 0x2900.

Start address	Number of registers	Register 1-12	MODBUS function code
0x2900	0x0C	k1~k6	0x03

Figure 51: Request frame to Get Customer Calibration Coefficients Command

Below is an example of request and response frames for getting Customer Calibration Coefficients command, assuming slave device address is 0x01, returned Customer Calibration Coefficients are K1=6.86,K2=-6.72,K3=0.04, K4=6.86,K5=-6.56,K6=-1.04 .

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x29	0x00	0x00	0x0C	0x4D	0x93

Figure 52: Request frame to Get Customer Calibration Coefficients Command

Definition	Device address	Function code	Number of bytes	Register value				CRC	
Byte	0	1	2	3-14		15-26		27	28
Value	0x01	0x03	0x0C	k1~k3		k4~k6		0xAB	0xF5

Figure 53: Response frame for Get Customer Calibration Coefficients Command

K1(3~6)				K2(7~10)				K3(11~14)				K4(15~18)			
0x1f	0x85	0xdb	0x40	0x3d	0x0a	0xd7	0xc0	0x0a	0xd7	0x23	0x3d	0x1f	0x85	0xdb	0x40
K5(19~22)				K6(23~26)											
0x85	0xeb	0xd1	0xc0	0xb8	0x1e	0x85	0xbf								

Figure 54: Registers definition for Customer Calibration Coefficients.

2.2.11 Get pH User Calibration Coefficients

Purpose: Get pH calibration coefficients K and B.

User calibration coefficients (K and B) can be read from 4 continuous MODBUS registers starting from address 0x1100.

Start address	Number of registers	Register 1-2	Register 3-4	MODBUS function code
0x1100	0x04	K	B	0x03

Figure 55: Register definition of Get pH User Calibration Coefficients Command

Below is an example of request and response frames for getting customer calibration coefficients from a device with slave address 0x01, assuming returned values are: K=1.0; B=0.0.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x11	0x00	0x00	0x04	0x41	0x35

Figure 56: Request frame to Get pH User Calibration Coefficient Command

Definition	Device address	Function code	Number of bytes	Register value		CRC	
Byte	0	1	2	3-6	7-10	11	12
Value	0x01	0x03	0x08	1.0	0.0	0x9E	0x12

Figure 57: Response frame for Get pH User Calibration Coefficient Command

Note: K and B are floating point numbers in little-endian storage mode

K(3-6)				B(7-10)			
0x00	0x00	0x80	0x3F	0x00	0x00	0x00	0x00

Figure 58: Registers for two coefficients K and B.

2.2.12 Set pH User Calibration Coefficients

Purpose: Set pH calibration coefficients K and B.

Customer coefficients (K and B) can be set at 4 continuous MODBUS registers starting from address 0x1100.

Start address	Number of registers	Register 1-2	Register 3-4	MODBUS function code
0x1100	0x04	K	B	0x10

Figure 59: Register definition of Set pH User Calibration Command

Below is an example of request and response frames for setting customer calibration coefficients, assuming slave address is 0x01, coefficients are K=1.0 and B=0.0.

Definition	Device address	Function code	Start address		Number of registers		Number of bytes	Register value		CRC	
Byte	0	1	2	3	4	5	6	7-10	11-14	15	16
Value	0x01	0x10	0x11	0x00	0x00	0x04	0x08	1.0	0.0	0x81	0xAE

Figure 60: Request frame to Set pH User Calibration Coefficient Command

Note: Coefficients K and B, floating point numbers in little-endian storage mode

K(7-10)				B(11-14)			
---------	--	--	--	----------	--	--	--

0x00	0x00	0x80	0x3F	0x00	0x00	0x00	0x00
------	------	------	------	------	------	------	------

Figure 61: Registers for two coefficients K and B

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x10	0x11	0x00	0x00	0x04	0xc4	0xf6

Figure 62: Response frame for Set Customer Calibration Coefficient Command

2.2.13 Get NH4+ User Calibration Coefficients

Purpose: Get NH4+ calibration coefficients K and B.

User calibration coefficients (K and B) can be read from 4 continuous MODBUS registers starting from address 0x3600.

Start address	Number of registers	Register 1-2	Register 3-4	MODBUS function code
0x3600	0x04	K	B	0x03

Figure 63: Register definition of Get NH4+ User Calibration Coefficients Command

Below is an example of request and response frames for getting customer calibration coefficients from a device with slave address 0x01, assuming returned values are: K=1.0; B=0.0.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x36	0x00	0x00	0x04	0x4B	0x81

Figure 64: Request frame to Get NH4+ User Calibration Coefficient Command

Definition	Device address	Function code	Number of bytes	Register value		CRC	
Byte	0	1	2	3-6	7-10	11	12
Value	0x01	0x03	0x08	1.0	0.0	0x9E	0x12

Figure 65: Response frame for Get NH4+ User Calibration Coefficient Command

Note: K and B are floating point numbers in little-endian storage mode

K(3-6)				B(7-10)			
0x00	0x00	0x80	0x3F	0x00	0x00	0x00	0x00

Figure 66: Registers for two coefficients K and B.

2.2.14 Set NH4+ User Calibration Coefficients

Purpose: Set NH4+ calibration coefficients K and B.

Customer coefficients (K and B) can be set at 4 continuous MODBUS registers starting from address 0x3600.

Start address	Number of registers	Register 1-2	Register 3-4	MODBUS function code
0x3600	0x04	K	B	0x10

Figure 67: Register definition of Set NH4+ User Calibration Command

Below is an example of request and response frames for setting NH4+ customer calibration coefficients, assuming slave address is 0x01, coefficients are K=1.0 and B=0.0.

Definition	Device address	Function code	Start address		Number of registers		Number of bytes	Register value		CRC	
Byte	0	1	2	3	4	5	6	7-10	11-14	15	16
Value	0x01	0x10	0x36	0x00	0x00	0x04	0x08	1.0	0.0	0x81	0xAE

Figure 68: Request frame to Set NH4+ User Calibration Coefficient Command

Note: Coefficients K and B, floating point numbers in little-endian storage mode

K(7-10)				B(11-14)			
0x00	0x00	0x80	0x3F	0x00	0x00	0x00	0x00

Figure 69: Registers for two coefficients K and B

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x10	0x36	0x00	0x00	0x04	0xc4	0xf6

Figure 70: Response frame for Set Customer Calibration Coefficient Command

2.2.15 Get NH3_N User Calibration Coefficients

Purpose: Get NH3_N calibration coefficients K and B.

User calibration coefficients (K and B) can be read from 4 continuous MODBUS registers starting from address 0x3400.

Start address	Number of registers	Register 1-2	Register 3-4	MODBUS function code
0x3400	0x04	K	B	0x03

Figure 71: Register definition of Get NH3_N User Calibration Coefficients Command

Below is an example of request and response frames for getting customer calibration coefficients from a device with slave address 0x01, assuming returned values are: K=1.0; B=0.0.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x34	0x00	0x00	0x04	0x4B	0x81

Figure 72: Request frame to Get NH3_N User Calibration Coefficient Command

Definition	Device address	Function code	Number of bytes	Register value		CRC	
Byte	0	1	2	3-6	7-10	11	12
Value	0x01	0x03	0x08	1.0	0.0	0x9E	0x12

Figure 73: Response frame for Get NH3_N User Calibration Coefficient Command

Note: K and B are floating point numbers in little-endian storage mode

K(3-6)				B(7-10)			
0x00	0x00	0x80	0x3F	0x00	0x00	0x00	0x00

Figure 74: Registers for two coefficients K and B.

2.2.16 Set NH3_N User Calibration Coefficients

Purpose: Set NH3_N calibration coefficients K and B.

Customer coefficients (K and B) can be set at 4 continuous MODBUS registers starting from

address 0x3400.

Start address	Number of registers	Register 1-2	Register 3-4	MODBUS function code
0x3400	0x04	K	B	0x10

Figure 75: Register definition of Set NH3_N User Calibration Command

Below is an example of request and response frames for setting NH3_N customer calibration coefficients, assuming slave address is 0x01, coefficients are K=1.0 and B=0.0.

Definition	Device address	Function code	Start address		Number of registers		Number of bytes	Register value		CRC	
Byte	0	1	2	3	4	5	6	7-10	11-14	15	16
Value	0x01	0x10	0x34	0x00	0x00	0x04	0x08	1.0	0.0	0x81	0xAE

Figure 76: Request frame to Set NH3_N User Calibration Coefficient Command

Note: Coefficients K and B, floating point numbers in little-endian storage mode

K(7-10)				B(11-14)			
0x00	0x00	0x80	0x3F	0x00	0x00	0x00	0x00

Figure 77: Registers for two coefficients K and B

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x10	0x34	0x00	0x00	0x04	0xc4	0xf6

Figure 78: Response frame for Set Customer Calibration Coefficient Command

2.2.17 Active Brush

Purpose: Make brush rotate. It is strongly recommend that brush should be active once power on.

MODBUS register 0x3100 is used.

Start address	Number of registers	MODBUS function code
0x3100	0x00	0x10

Figure 79: Register definition of active brush Command

Below is an example of request and response frames for a device with slave address 0x01 to active brush.

Definition	Device address	Function code	Start address		Number of registers		Number of bytes	CRC	
Byte	0	1	2	3	4	5	6	7	8
Value	0x01	0x10	0x31	0x00	0x00	0x00	0x00	0x74	0x94

Figure 80: Request frame to Active brush Command

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x10	0x31	0x00	0x00	0x00	0xc4	0xf5

Figure 81: Response frame to Active brush Command

2.2.18 Set Brush Interval of time

Purpose: Set the interval of time for brush between each rotation, the unit is minute.

The interval of time can be set at 1 MODBUS registers starting from address 0x3200.

Start address	Number of registers	Register 1	MODBUS function code
0x3200	0x01	Interval of time(min)	0x10

Figure 82: Register definition of Set Brush Interval of time Command

Below is an example of request and response frames for setting brush interval of time, assuming slave address is 0x01, time is 10min.

Definition	Device address	Function code	Start address		Number of registers		Number of bytes	Register value		CRC	
Byte	0	1	2	3	4	5	6	7	8	15	16
Value	0x01	0x10	0x32	0x00	0x00	0x01	0x02	0x0a	0x00	0xb3	0x33

Figure 83: Request frame to Set Brush Interval of time Command

Note: Time in little-endian storage mode

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x10	0x32	0x00	0x00	0x01	0x0f	0x71

Figure 84: Response frame to Set Brush Interval of time Command

2.2.19 Get Brush Interval of time

Purpose: Get the interval of time for brush between each rotation, default time is 30 min.

The interval of time can be read from 1 MODBUS registers starting from address 0x3200.

Start address	Number of registers	Register 1	MODBUS function code
0x3200	0x01	Interval of time(min)	0x03

Figure 85: Register definition of Get Brush Interval of time Command

Below is an example of request and response frames for getting brush interval of time from a device with slave address 0x01, assuming returned time is 30min.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0x01	0x03	0x32	0x00	0x00	0x01	0x8a	0xb2

Figure 86: Request frame to Get Brush Interval of time Command

Definition	Device address	Function code	Number of bytes	Register value		CRC	
Byte	0	1	2	3	4	5	6
Value	0x01	0x03	0x02	0x1E	0x00	0xb1	0xe4

Figure 87: Response frame to Get Brush Interval of time Command

2.2.20 Get Slave Device ID

Purpose: Get current MODBUS slave address to a sensor probe. Use 0xFF as fixed Device address.

Sensor probe slave address can be read from MODBUS registers 0x3000.

Start address	Number of registers	Register 1	MODBUS Function code
0x3000	0x01	Current Slave address	0x10

Figure 88: Get slave ID command

Below is an example of request and response frames for getting slave device id, assuming returned address is 0x03.

Definition	Device address	Function code	Start address		Number of registers		CRC	
Byte	0	1	2	3	4	5	6	7
Value	0xFF	0x03	0x30	0x00	0x00	0x01	0x9E	0xD4

Figure 89: Request frame of get slave device ID comment

Definition	Device address	Function code	Number of bytes	Register value		CRC	
Byte	0	1	2	3	4	5	6
Value	0xFF	0x03	0x02	0x03	0x00(reserve)	0x91	0x60

Figure 90: Response frame of get slave device ID comment

3 Procedure to get NH3_N value

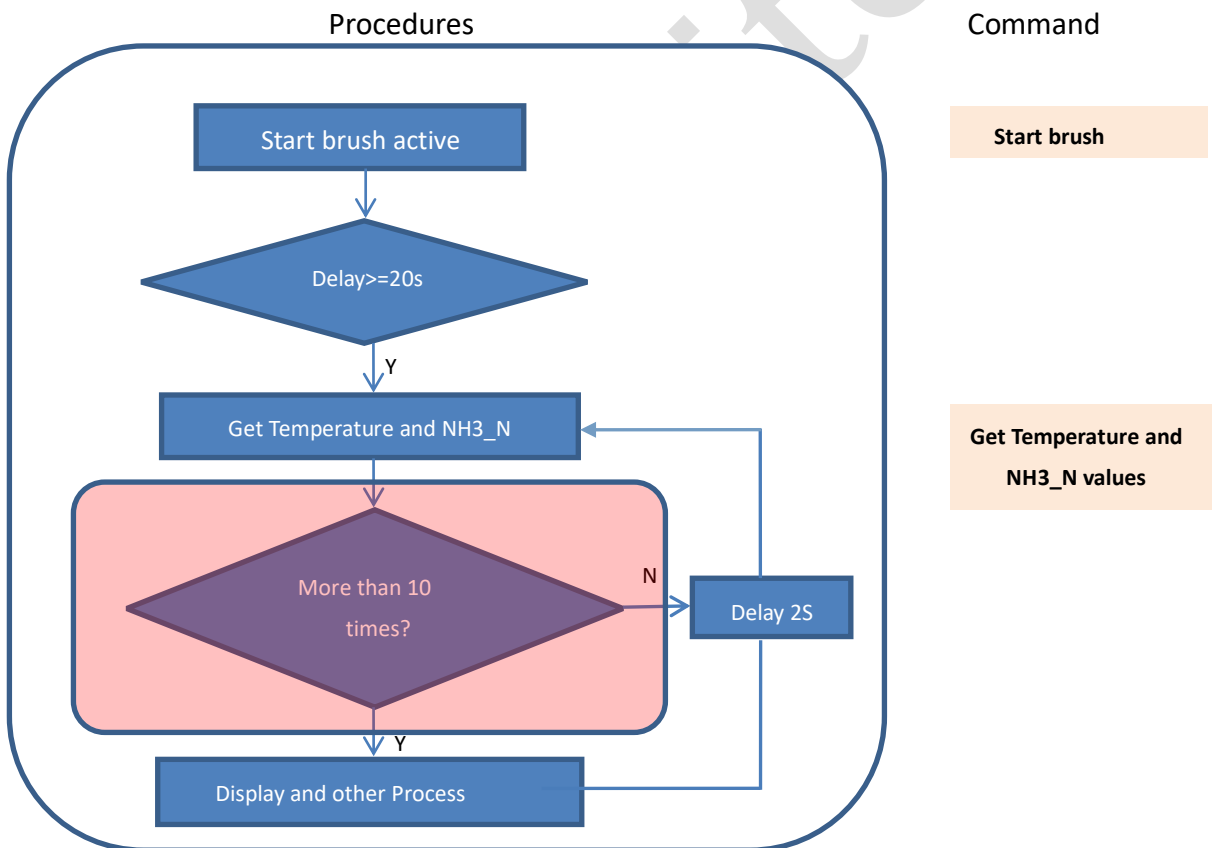


Figure 91: Flow chart to get NH3_N measurement

- **Start brush active** – make the brush active once power on , then the brush will work at the set interval time.
- **Get temperature and NH3_N values** – Get measurement results including temperature (°C)

and NH3_N (mg/L) after 20 seconds of brush active.

Note: Please pay attention to highlighted portion (red) in the flow chart above. It's highly recommended that customers get an average NH3_N results after 10 consecutive measurements, then perform display or other process.

Yosemite