



**Trinity College Dublin**

Coláiste na Tríonóide, Baile Átha Cliath

The University of Dublin

School of Engineering

Electronic Engineering

# MERIT.jl: Julia's Version

Aaron Dinesh

Supervisor: Associate Prof. Declan O'Loughlin

March 31, 2024

A Final Year Project submitted in partial fulfilment  
of the requirements for the degree of  
MAI (Electronic and Computer Engineering)

# Declaration

I hereby declare that this Final Year Project is entirely my own work and that it has not been submitted as an exercise for a degree at this or any other university.

I have read and understand the plagiarism provisions in the General Regulations of the University Calendar for the current year, found at <http://www.tcd.ie/calendar>.

I have completed the Online Tutorial on avoiding plagiarism 'Ready Steady Write', located at <http://tcd-ie.libguides.com/plagiarism/ready-steady-write>.

I consent/do not consent to the examiner retaining a copy of the thesis beyond the examining period, should they so wish (EU GDPR May 2018).

I agree that this thesis will not be publicly available, but will be available to TCD staff and students in the University's open access institutional repository on the Trinity domain only, subject to Irish Copyright Legislation and Trinity College Library conditions of use and acknowledgment. **Please consult with your supervisor on this last item before agreeing, and delete if you do not consent**

Signed: Aaron Dinesh Date: March 31, 2024

# Abstract

MERIT aims to provide a software framework that is robust, easy to use and performant. It implements a variety of microwave imaging algorithms and a myriad of helper functions, all while leveraging the powerful features available in Julia. MERIT.jl also implements a “Scan” abstract datatype which allows users to subtype their own specialized datatype. Organizing the datatypes in this way means that MERIT.jl plays very well with Julia’s own type hierarchy and also the other language features that depend on this. To encourage type safety, MERIT.jl implements a lightweight Points class which allows for efficient processing of coordinate points. In this way, collections of points won’t simply be a matrix of Floats or Ints instead, they would be a Vector of the Points type. In this way, the Julia compiler will throw an error when Points aren’t passed in the right argument, instead of providing a wrong output.

# Acknowledgements

Thanks, Everyone!

# List of Figures

1.1	Example of a Fully Multistatic Configuration (Top-Down) . . . . .	2
1.2	The MARIA M4 and M5 system. (a) The MARIA M4 antenna array. (b) The M4 in a clinical setting. (c) The integrated M5 package [2] . . . . .	3
1.3	The Wavelia System [4] . . . . .	4
1.4	The Leveled Multistatic Approach of Wavelia [4] . . . . .	4
1.5	The TSAR Prototype [8] . . . . .	6

# Contents

<b>Introduction</b>	<b>1</b>
<b>Background</b>	<b>2</b>
1.1 Literature Review . . . . .	2
1.1.1 MARIA M4 . . . . .	2
1.1.2 Wavelia . . . . .	3
1.1.3 TSAR . . . . .	5

# Introduction

MERIT.jl was motivated by a need to streamline the development process for new imaging algorithms. Currently, any researcher who wants to code a novel microwave imaging algorithm not only has to code the algorithm itself but also has to code all the helper functions required to produce an image. All this time fixing bugs subtracts from the time that could be spent fine-tuning the algorithm and choosing an optimal parameter set. The use of such open-source software has seen widespread use in a myriad of fields. PsychoPy and PsyToolkit are two such frameworks that revolutionized the field of psychological sciences. By implementing commonly used functions and scripts, they have allowed researchers to design and run experiments in a matter of hours. It has also allowed researchers who have little to no programming experience to get up and running with automated data processing, thereby allowing them to focus more on the quality of their experiment. [1]

The use of microwaves in imaging has started to gain interest amongst the medical community as an alternative and safer form of imaging when compared to more traditional methods such as X-rays. Clinical trials such as the “MARIA M4” system has proven that such microwave-based methods are more comfortable and are a viable alternative to current mammograms [2]. Mammography is not the only area where this imaging modality is being trailed. It is seeing use in areas such as traumatic brain injury detection, bone degradation and tumor detection [3]. While the hardware has proved effective, the software leaves a lot to be desired.

That is where this project comes in. MERIT.jl aims to be an easy-to-use, extensible and featureful library. The goal being that anyone, regardless of coding experience, would be able to quickly create a script that allows them to process and visualize the scan data they have collected. The following sections will contain:

- A literature review on the existing microwave imaging systems
- A look into existing microwave imaging frameworks
- A discussion about the design choices and Julia features that are included
- An examination of the results and possible future work

# Background

## 1.1 Literature Review

In order to understand the design requirements of the library, a literature review needed to be performed. The scope was narrowed down to 3 systems that showed promise and were broadly representative of the antenna configuration that future systems would adopt. Most systems will adopt one of the following setups

1. Monostatic
2. Leveled Multistatic
3. Fully Multistatic

These terms relate to the position of antennas around the breast tissue and how the resulting scan data would be structured.

### 1.1.1 MARIA M4

The first system we will look at is the MARIA M4 system developed by Preece et al within the Electrical and Engineering Department of the University of Bristol [2]. This is the 4th iteration in a series of MARIA systems that evolved from a system of 16 UWB antennas to 60 antennas in the current system. These all operate in a multistatic configuration, meaning that any antenna in the array can listen to any other antenna in the array, an example of which can be seen in Figure 1.1. This figure shows a top-down view, however, one can imagine this being generalized to a hemisphere of antennas around the breast.

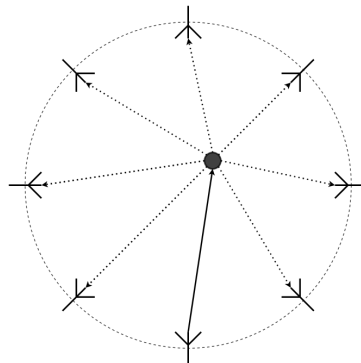


Figure 1.1: Example of a Fully Multistatic Configuration (Top-Down)



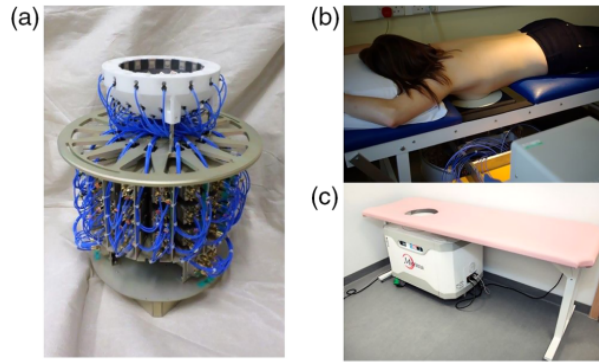


Figure 1.2: The MARIA M4 and M5 system. (a) The MARIA M4 antenna array. (b) The M4 in a clinical setting. (c) The integrated M5 package [2]

As stated before, the MARIA M4 system makes use of the UWB spectrum over a frequency range of 3.0 to 8.0 GHz. A VNA was used to step through the frequencies and collect the scans from the antenna. The system exploits the inherent symmetry in the antenna reciprocity to halve the number of channels (made of a transmitting and receiving antenna) collected, thereby speeding up the scan time. For the MARIA M4 system, this equates to a 1770 reduction in the number of channels collected. Figure 1.2, shows the antenna array used in the M4 system (a), as well as the M5 system (c) which is an integrated package.

The team scanned 86 participants, with a mean age of 51.4 and a range of 24 - 78 years old. The M4 system showed a sensitivity of 74% (64/86) when compared with the "gold-standard" of an ultrasound. The "sensitivity" was determined based on the ability of the M4 system to localize a lesion as it correlated with the location in the ultrasound image. The research team also divided the group into pre-/peri- and post- menopausal women and found that the sensitivity was 75% and 73% respectively. However, the reliability of these results are called into question when considering the sample size of the study. Given a sample size of 86, and assuming a normal distribution and that the results are statistically significant ( $p < 0.05$ ,  $Z = 1.96$ ), a 7.11% margin of error was calculated. While this may not be enough to conclusively prove that the M4 system is a viable alternative to Mammograms, it is enough to show promise. With a larger sample size, this margin of error could be narrowed further.

### 1.1.2 Wavelia

The second system that was considered was the Wavelia Microwave Breast Imaging System developed by MVG Industries [4]. The Wavelia system integrates the imaging system as well as the examination bed into one complete package (Figure 1.3). The integrated package makes the Wavelia system an appealing choice for some hospitals, however, its large size may be a barrier to adoption in some facilities where space is a premium.

Like in the MARIA M4 system, patients lie in a prone position and place their breasts in the circular cutouts on the bed. The system then begins to create a 3D reconstruction of the exterior of the breast using a stereoscopic camera. This also allows for the breast volume to be explicitly calculated rather than being inferred like in the MARIA system. The Wavelia makes use of the UWB spectrum when imaging the breast, although they opt for a narrower frequency range of 0.5 - 4.0 GHz compared to the 3.0 - 8.0 GHz range of the MARIA system. The antenna configuration, unlike the MARIA system, is an array of 18 Vivaldi-type probes



Figure 1.3: The Wavelia System [4]

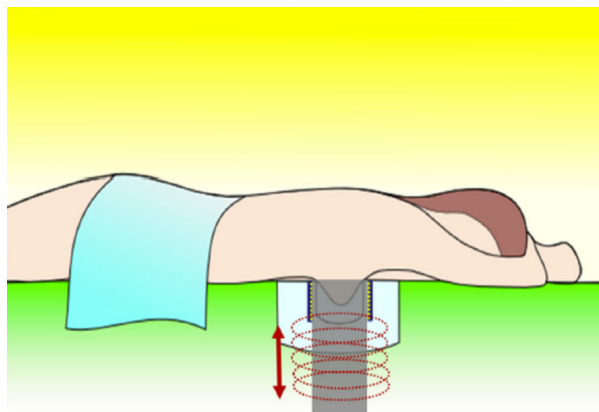


Figure 1.4: The Levelled Multistatic Approach of Wavelia [4]

arranged in a concyclic manner on a horizontal plane. These antennas operate in a Multistatic manner and image the breast in sections parallel to the coronal plane. The entire antenna assembly moves downwards in 5mm intervals to image the entire breast (Figure 1.4). This is a leveled multistatic system as opposed to the fully multistatic system in the MARIA M4. This leveled multistatic approach has the benefit of a theoretically infinite vertical resolution. If the radiologist wanted a finer resolution along the coronal plane, they would just have to tweak the array vertical step size, rather than having to manufacture an entirely new antenna array, like in the MERIT system. This leveled approach also allows the parameters of the reconstruction algorithm to be easily changed based on the particular section of the breast that we are imaging. The fully multistatic approach, however, would need significant additional logic in the post-processing steps to determine which channels are coplanar with a particular section.

The Wavelia paper [4] conducted a feasibility study on 25 female participants. While the results aren't statistically significant, they do demonstrate the strengths of the Wavelia system. 11 of the participants had a biopsy confirmed carcinoma and out of these, the Wavelia system detected 9 lesions, with 7 being located to the appropriate region. Overall the system detected

an abnormality in 21 of the 24 participants, leading to a sensitivity of 87.5%. The researchers do note some limitations of the Wavelia system, namely it can't detect any lesions smaller than 10mm. This is significant since the size of the detected lesion plays a big factor when deciding whether a lesion is cancerous or not. Another limitation of the system is that breast sizes that are too small cannot be scanned in any great detail by the Wavelia system. Due to the patients being in the prone position, their breast tissue needs to hang down far enough to have multiple sections of their breast be imaged by the antenna array. The researchers are working on a subsequent system that should address all the aforementioned limitations. Overall the participants had a positive outlook on the system. 23 out of the 25 women said that they would recommend the procedure to other women and all of the women agreed that the information provided was clear and well understood.

### 1.1.3 TSAR

The third and final system considered for the project was the TSAR system [5]. Standing for Tissue Sensing Adaptive Radar, this system was developed by the University of Calgary to address some of the shortcomings of the previous two systems. In the MERIT and Wavelia systems, reflections from the skin can muddy the data and can lead to artifacts in the final image. In order to get around this, both systems take an additional scan, offset by a fixed rotational amount in the coronal plane. The idea being, that any reflections that appear on the first scan would appear with similar amplitude in the second scan at the same time position, while the tumor would show in a different place, provided that the tumor doesn't lie on the axis of rotation. This method is known as Rotational Subtraction [6]. The TSAR system, on the other hand, makes use of an adaptive algorithm that instead estimates the skin response at an antenna as the weighted sum of the responses from the neighboring antennas. This skin response can then be subtracted from the current antenna to remove the reflection artifacts [7].

Like the previous two systems, patients lie in the prone position on the examination table, with their breast being submerged in an immersion liquid. However, unlike the previous two systems, the TSAR operates in a monostatic configuration. In this setup, there is only one antenna that acts as both the transmitting and the receiving antenna. This antenna, usually fixed on some type of rotating apparatus, would rotate around the breast to image a section. It would then step vertically by a fixed amount and repeat the previous step, eventually imaging the entire breast. The TSAR system also operates on a much wider section of the UWB spectrum, from 50 MHz to 15 GHz, with the frequency data being collected by a VNA. The system also makes use of a laser in order to help with the 3D reconstruction of the breast during post-processing. The prototype setup can be seen in Figure 1.5

The benefit of the monostatic configuration is that the number of antenna locations per row and the number of rows are parameters that can be tweaked depending on whether the radiologist would want a quicker scan or higher precision. One can imagine the scenario of a rapid screening center as part of a national screening program where the speed of the scan is valued over the precision of the scan. As such this provides a notable benefit over the previous two systems. The clinical trial conducted by this study was extremely limited, only including 8 successfully imaged patients. Due to the low sample size, one can't reliably say whether this system and its adaptive reflection-suppressing algorithm can outperform the other two systems in terms of accuracy, although the TSAR system does show promise.



Figure 1.5: The TSAR Prototype [8]

# Bibliography

- [1] G. Stoet, PsyToolkit Testimonials, Std. [Online]. Available: [https://www.psytoolkit.org/#\\_testimonials](https://www.psytoolkit.org/#_testimonials)
- [2] A. W. Preece, I. Craddock, M. Shere, L. Jones, and H. L. Winton, "MARIA M4: Clinical evaluation of a prototype ultrawideband radar scanner for breast cancer detection." vol. 3, no. 3, p. 033502.
- [3] N. Alsbou, K. Cisse, C. Cox, M. Akinbola, and I. Ali, "Medical Imaging System Design using Microwave Antennas and Portable Platform," in 2023 IEEE 17th International Symposium on Medical Information and Communication Technology (ISMICT). IEEE, pp. 1–5. [Online]. Available: <https://ieeexplore.ieee.org/document/10152069/>
- [4] B. M. Moloney, P. F. McAnena, S. M. Elwahab, A. Fasoula, L. Duchesne, J. D. Gil Cano, C. Glynn, A. O'Connell, R. Ennis, A. J. Lowery, and M. J. Kerin, "The Wavelia Microwave Breast Imaging system-tumour discriminating features and their clinical usefulness." vol. 94, no. 1128, p. 20210907.
- [5] E. C. Fear, J. Bourqui, C. Curtis, D. Mew, B. Docktor, and C. Romano, "Microwave Breast Imaging With a Monostatic Radar-Based System: A Study of Application to Patients," vol. 61, no. 5, pp. 2119–2128.
- [6] M. Klemm, I. Craddock, J. Leendertz, A. Preece, and R. Benjamin, "Improved Delay-and-Sum Beamforming Algorithm for Breast Cancer Detection," vol. 2008.
- [7] B. Maklad, C. Curtis, E. Fear, and G. Messier, "Neighborhood-Based Algorithm to Facilitate the Reduction of Skin Reflections in Radar-Based Microwave Imaging," vol. 39, pp. 115–139.
- [8] J. Bourqui, J. Sill, and E. Fear, "A Prototype System for Measuring Microwave Frequency Reflections from the Breast," vol. 2012, p. 851234.