

# A Pseudo Plane-wave Gravitational Calibrator for Gravitational Wave Observatories

M.P. Ross,<sup>1,\*</sup> J.H. Gundlach,<sup>1</sup> C. Weller,<sup>1</sup> E.G. Adelberger,<sup>1</sup> Jeff Kissel,<sup>2</sup> Timesh Mistry,<sup>3</sup> and Laurence Datrier<sup>4</sup>

<sup>1</sup>*Center for Experimental Nuclear Physics and Astrophysics,  
University of Washington, Seattle, Washington, 98195, USA*

<sup>2</sup>*LIGO Hanford Observatory, Richland, WA 99352, USA*

<sup>3</sup>*The University of Sheffield, Sheffield S10 2TN, UK*

<sup>4</sup>*SUPA, University of Glasgow, Glasgow G12 8QQ, UK*

Gravitational calibration has recently gained interest as a possible improvement to gravitational wave observatories. The precision of existing gravitational calibrators are limited by their dependence on the relative position between the calibrators and the test masses. Here we present a novel geometry consisting of four quadrupole rotors placed at the vertices of a square centered on the test mass. The phases and rotation directions are selected to produce a pseudo plane-wave sinusoidal gravitational acceleration with amplitude of  $376.19 \text{ fm/s}^2$ . This acceleration has minimal positioning dependence and can yield  $\sim 0.1\%$  acceleration amplitude uncertainty for  $\sim 1 \text{ cm}$  test mass positioning uncertainty. In addition, these rotors have significant engineering and safety benefits due to their small size and eliminates the torques acting on the test mass.

## I. INTRODUCTION

Gravitational wave astronomy has blossomed into a novel method to observe the universe. The number of gravitational wave observations is expected to grow substantially in the coming years with the continued operation of the LIGO [1] and Virgo [2] interferometers as well the future addition of LIGO-India [3] and the further improvements of KAGRA [4].

These interferometers must be precisely calibrated in order to accurately interpret gravitational wave signals. Whether for binary merger parameter estimation [5], cosmological measurements [6, 7], or searches for deviations from general relativity [8], the strain readouts of the observatories must be precisely and accurately calibrated.

Thus far, the calibration of the current observatories has been accomplished with photon pressure [9]. These photon calibration systems have yielded absolute calibrations with  $\sim 0.5\%$  uncertainty and have acted as versatile calibration tools.

Calibrating with a gravitationally induced strain has long been suggested as an alternative calibration technique [10–15] and has recently been explored at many of the observatories [16–19]. Gravitational calibration has the promise of improving the absolute calibration of the observatories by achieving higher-precision injections. Additionally, gravitational calibrators can work in concert with photon calibrators to yield a combined calibration with lower uncertainty.

The geometries explored with current gravitational calibrators [16–19] produce accelerations that have large dependence on the radial distance,  $r$ , between the rotor and the test mass. The acceleration is typically proportional to  $\sim 1/r^{l+2}$  where  $l$  is the order of the dominate mass-multipole moment. For example, a rotor with a quadrupole mass distribution ( $l = 2$ ) will follow  $\sim 1/r^4$ .

This strong positioning dependence causes the performance of the absolute calibration to be limited by the precision of the positioning measurements.

Here, we present a novel geometry consisting of four quadrupole rotors that produces a pseudo plane-wave gravitational acceleration. This geometry produces an acceleration which has minimal first-order dependence on the position of the rotors allowing for improved calibration precision with limited positioning precision. Additionally, this geometry eliminates the torques acting on the test mass and eases much of the engineering and safety concerns of previous rotors.

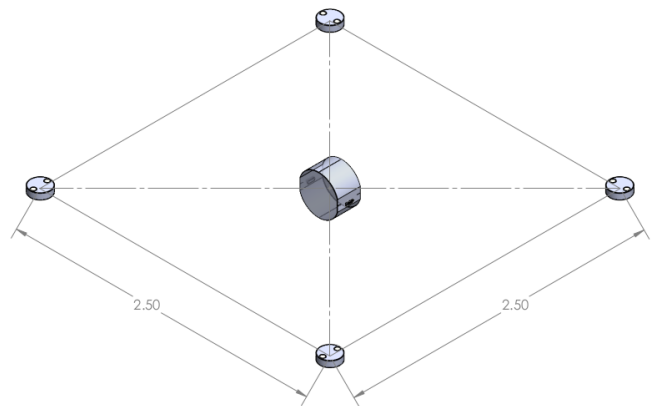


FIG. 1. A rendering of the geometry of the rotors with the test mass at the center of the square.

## II. GEOMETRY

The pseudo plane-wave calibrator consists of four identical rotors placed at the vertices of a 2.5 meter sided square centered on the test mass. Figure 1 shows a rendering of the geometry. The rotors are designed with the

\* mpross2@uw.edu

similar dimensions as the LIGO NCal [19] but without a hexapole mass arrangement. Each rotor is a 17 cm diameter, 5 cm tall aluminum disk with two holes cut at a radius of 6 cm separated by  $90^\circ$ . These holes are filled in with 4 cm diameter, 5 cm tall tungsten cylinders which produce a quadrupole mass distribution. The parameters of the geometry are displayed in Table I.

The parameters that are common with the LIGO NCal are assigned uncertainties equal to what was previously achieved [19]. The rest of the parameters are assigned uncertainties based on what is reasonably achievable with

standard measurement techniques. For example, since the rotors would be outside the interferometer's vacuum system, their positions can be readily measured to the mm-precision with standard surveying equipment.

The relative phases of the rotors and the rotation directions are set to achieve pseudo plane-wave nature. The four rotor with a positive x-coordinate are rotated by  $90^\circ$  from the rotors with negative x-coordinate. Additionally, the rotors with positive y-coordinate rotate clockwise while those with negative y-coordinates rotate counter-clockwise.

Parameter	Mean	Uncertainty
Cylinder Mass	1 kg	0.3 g
Cylinder Radius	2 cm	$2.5 \mu\text{m}$
Cylinder Length	5 cm	$5 \mu\text{m}$
Quadrupole Radius	6 cm	$5 \mu\text{m}$
Test Mass	40 kg	10 g
Test Mass Length	200 mm	0.1 mm
Test Mass Radius	170 mm	0.05 mm
Test Mass Flat Width	327 mm	0.05 mm
Rotor Positions	$(\pm 1.25 \text{ m}, \pm 1.25 \text{ m}, 0 \text{ m})$	(1 mm, 1 mm, 1 mm)
Test Mass Position	(0 m, 0 m, 0 m)	(1 cm, 1 cm, 1 cm)

TABLE I. Parameters describing the rotors, the test mass, and their respective positions.

### III. ENGINEERING SIMPLICITY

### IV. PSEUDO PLANE-WAVE NATURE

To verify the performance of such a rotor array, we simulated the system with a finite-element analysis using the *PointGravity* algorithms of the `newt` libraries [20, 21]. This simulation breaks each of the rotor cylinders and the test mass into independent clouds of point masses. The force between each pair of point masses, one from the rotors and the other from the test mass, is calculated. The forces from the individual pairs of point masses is then summed to yield the acceleration in all three directions. We extract only the x-acceleration as this is the primary sensitive direction of the interferometer.

The superposition of the gravitational fields from the four rotors produces an oscillating gravitational acceleration field which at the center of the square is only in the x-direction and has an amplitude of  $376.19 \text{ fm/s}^2$ . This amplitude corresponds to a strain of  $2.6 \times 10^{-21}$  at 30 Hz for a 4-km long interferometer. Note that although the acceleration amplitude is frequency independent, the strain amplitude will follow  $\sim 1/f^2$ . The ac-

celeration field changes weakly with deviations from the center of the square (i.e. a pseudo plane-wave). The percentage change in acceleration amplitude verse offset from the center of the square is shown in Figure 2 for offsets in each direction. A relatively large offset of 10 cm in any direction changes the acceleration by  $< 2\%$ . Additionally, the change in amplitude is well-described by a parabola for small offsets displaying the second-order nature of this effect.

Since the rotor array is in-plane and symmetric about the x-z plane, the rotors apply no net torque on the test mass. If the array is out-of-plane then the test mass would experience a torque about the y-axis. Similarly, if the array is asymmetric it would apply a z-axis torque. Such torques are common in existing gravitational calibrators and can substantially impact the precision of the subsequent calibrations.

### V. NUMERICAL UNCERTAINTY ANALYSIS

Since the performance of such a calibrator does not only depend on the test mass offset, we performed a

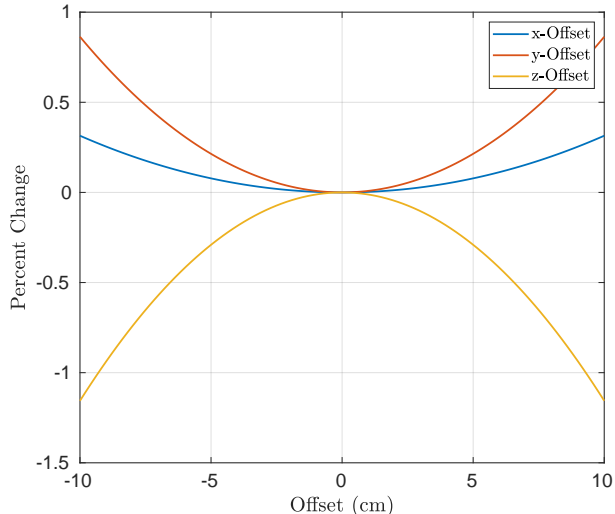


FIG. 2. The percentage change of acceleration amplitude with a test mass offset from the center of the square.

Monte Carlo simulation of the applied acceleration to accounting for the set of parameters which describe the cali-

brator. We model each parameter as a Gaussian distribution centered on the mean listed in Table I with  $\sigma$ -value equal to the uncertainty. The acceleration of the test mass is then calculated with parameters sampled from these distributions. This is repeated 2000 times to yield a distribution of the gravitational acceleration, shown in Figure 3, which takes into account all non-linearities and degeneracies.

The simulation yields an injected acceleration of  $a = 376.19 \pm 0.47 \text{ fm/s}^2$  (0.12 %) where the central value is the mean and the uncertainty is the 68%-interval. To assess how each parameter contributes to this total uncertainty, the acceleration uncertainty was recomputed with only one parameter varying. This was then repeated for each parameter to yield the results in Table II. All four rotor positions were simultaneously varied in all three directions and the test mass position was also varied in all three directions.

Table II shows the acceleration uncertainty is strongly dominated by the rotor positions with the test mass position contribution being 3.5 times smaller. This contribution may be further reduced with a precision machined mounting frame for the rotors or with higher precision surveying than is assumed here.

Parameter	Mean	Uncertainty	Fractional Contribution
Cylinder Mass	1 kg	0.3 g	$3.70 \times 10^{-4}$
Cylinder Radius	2 cm	$2.5 \mu\text{m}$	$2.93 \times 10^{-8}$
Cylinder Length	5 cm	$5 \mu\text{m}$	$4.45 \times 10^{-8}$
Quadrupole Radius	6 cm	$5 \mu\text{m}$	$2.07 \times 10^{-4}$
Test Mass	40 kg	10 g	$2.95 \times 10^{-4}$
Test Mass Length	200 mm	0.1 mm	$1.01 \times 10^{-6}$
Test Mass Radius	170 mm	0.05 mm	$1.53 \times 10^{-6}$
Test Mass Flat Width	327 mm	0.05 mm	$2.55 \times 10^{-15}$
Rotor Positions	$(\pm 1.25 \text{ m}, \pm 1.25 \text{ m}, 0 \text{ m})$	(1 mm, 1 mm, 1 mm)	$9.54 \times 10^{-4}$
Test Mass Position	(0 m, 0 m, 0 m)	(1 cm, 1 cm, 1 cm)	$1.56 \times 10^{-4}$
Quadrature Sum			$1.10 \times 10^{-3}$

TABLE II. Individual uncertainty contributions for the input parameters of the simulation.

## VI. CONCLUSION

We have described an four-rotor gravitational calibrator that causes a psuedo-plane wave acceleration field. Simulation of the acceleration amplitude uncertainty shows that such a system can achieve  $\sim 0.1\%$  precision absolute calibration injections. This is approximately an order of magnitude improvement over previ-

ously deployed geometries.[19]

Gravitational calibration is a promising avenue for high precision absolute calibration of gravitational wave observatories. By deploying arrays which minimize the first-order contributions of the applied gravitational field around the test mass, such calibrators may exceed the performance of excising calibration techniques.

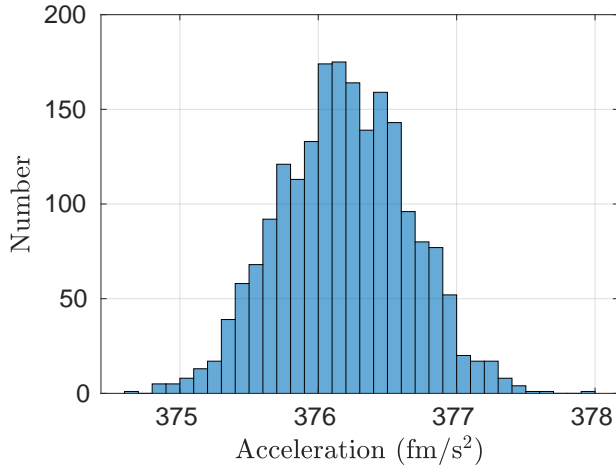


FIG. 3. Distribution of predicted accelerations.

## ACKNOWLEDGMENTS

Participation from the University of Washington, Seattle, was supported by funding from the NSF under Awards PHY-1607385, PHY-1607391, PHY-1912380, and PHY-1912514.

- 
- [1] J. Aasi et al. Advanced LIGO. *Classical and Quantum Gravity*, 32(7):074001, mar 2015. doi:10.1088/0264-9381/32/7/074001. URL <https://doi.org/10.1088/0264-9381/32/7/074001>.
  - [2] F Acernese et al. Advanced Virgo: a second-generation interferometric gravitational wave detector. *Classical and Quantum Gravity*, 32(2):024001, Dec 2014. doi:10.1088/0264-9381/32/2/024001. URL <https://doi.org/10.1088/0264-9381/32/2/024001>.
  - [3] M Saleem, Javed Rana, V Gayathri, Aditya Vijaykumar, Srashti Goyal, Surabhi Sachdev, Jishnu Suresh, S Sudhagar, Arunava Mukherjee, Gurudatt Gaur, Bangalore Sathyaprakash, Archana Pai, Rana X Adhikari, P Ajith, and Sukanta Bose. The science case for LIGO-india. *Classical and Quantum Gravity*, 39(2):025004, dec 2021. doi:10.1088/1361-6382/ac3b99. URL <https://doi.org/10.1088/1361-6382/ac3b99>.
  - [4] T Akutsu, M Ando, K Arai, Y Arai, S Araki, A Araya, N Aritomi, H Asada, Y Aso, S Atsuta, et al. Kagra: 2.5 generation interferometric gravitational wave detector. *NATURE ASTRONOMY*, 3(1):35, 2019.
  - [5] Rich Abbott, TD Abbott, S Abraham, F Acernese, K Ackley, A Adams, C Adams, RX Adhikari, VB Adya, C Affeldt, et al. Population properties of compact objects from the second LIGO-virgo gravitational-wave transient catalog. *arXiv preprint arXiv:2010.14533*, 2020. URL <https://arxiv.org/abs/2010.14533>.
  - [6] BP Abbott, R Abbott, TD Abbott, S Abraham, F Acernese, K Ackley, C Adams, RX Adhikari, VB Adya, C Affeldt, et al. A gravitational-wave measurement of the hubble constant following the second observing run of advanced LIGO and virgo. *The Astrophysical Journal*, 909(2):218, 2021. URL <https://iopscience.iop.org/article/10.3847/1538-4357/abdcb7/>.
  - [7] LIGO Scientific Collaboration, Virgo Collaboration, 1M2H Collaboration, Dark Energy Camera GW-EM Collaboration, DES Collaboration, DLT40 Collaboration, Las Cumbres Observatory Collaboration, VIN-ROUGE Collaboration, MASTER Collaboration, et al. A gravitational-wave standard siren measurement of the hubble constant. *Nature*, 551(7678):85–88, 2017. URL <https://www.nature.com/articles/nature24471>.
  - [8] R Abbott, TD Abbott, S Abraham, F Acernese, K Ackley, A Adams, C Adams, RX Adhikari, VB Adya, C Affeldt, et al. Tests of general relativity with binary black holes from the second LIGO-virgo gravitational-wave transient catalog. *arXiv preprint arXiv:2010.14529*, 2020. URL <https://arxiv.org/abs/2010.14529>.
  - [9] S Karki, D Tuyenbayev, S Kandhasamy, BP Abbott, TD Abbott, EH Anders, J Berliner, J Betzwieser, C Cahillane, L Canete, et al. The advanced ligo photon calibrators. *Review of Scientific Instruments*, 87(11):114503, 2016. URL <https://doi.org/10.1063/1.4967303>.
  - [10] Hiromasa Hirakawa, Kimio Tsubono, and Katsunobu Oide. Dynamical test of the law of gravitation. *Nature*, 283(5743):184–185, 1980. URL <https://www.nature.com/articles/283184a0>.
  - [11] Kazuaki Kuroda and Hiromasa Hirakawa. Experimental test of the law of gravitation. *Physical Review D*, 32(2):342, 1985. URL <https://doi.org/10.1103/PhysRevD.32.342>.
  - [12] Norikatsu Mio, Kimio Tsubono, and Hiromasa Hirakawa. Experimental test of the law of gravitation at small distances. *Physical Review D*, 36(8):2321, 1987. URL <https://doi.org/10.1103/PhysRevD.36.2321>.
  - [13] Pia Astone, M Bassan, S Bates, R Bizzarri, P Bonifazi, R Cardarelli, G Cavallari, E Coccia, A Degasperis, D De Pedis, et al. Evaluation and preliminary measurement of the interaction of a dynamical gravitational near field with a cryogenic gravitational wave antenna. *Zeitschrift für Physik C Particles and Fields*, 50(1):21–29, 1991. URL <https://doi.org/10.1007/BF01558552>.
  - [14] P Astone, M Bassan, R Bizzarri, P Bonifazi, L Brocco, P Carelli, E Coccia, C Cosmelli, A Degasperis, S Frasca, et al. Experimental study of the dynamic newtonian field with a cryogenic gravitational wave antenna. *The European Physical Journal C-Particles and Fields*, 5

- (4):651–664, 1998. URL <https://doi.org/10.1007/s100529800987>.
- [15] L Matone, P Raffai, S Márka, R Grossman, P Kalmus, Z Márka, J Rollins, and V Sannibale. Benefits of artificially generated gravity gradients for interferometric gravitational-wave detectors. *Classical and Quantum Gravity*, 24(9):2217–2229, apr 2007. doi: 10.1088/0264-9381/24/9/005. URL <https://doi.org/10.1088/0264-9381/24/9/005>.
- [16] D Estevez, B Lieunard, F Marion, B Mours, L Rolland, and D Verkindt. First tests of a newtonian calibrator on an interferometric gravitational wave detector. *Classical and Quantum Gravity*, 35(23):235009, nov 2018. doi: 10.1088/1361-6382/aae95f. URL <https://doi.org/10.1088/1361-6382/aae95f>.
- [17] Dimitri Estevez, Benoît Mours, and Thierry Pradier. Newtonian calibrator tests during the virgo o3 data taking. *Classical and Quantum Gravity*, 2021. URL <https://iopscience.iop.org/article/10.1088/1361-6382/abe2da>.
- [18] Yuki Inoue, Sadakazu Haino, Nobuyuki Kanda, Yujiro Ogawa, Toshikazu Suzuki, Takayuki Tomaru, Takahiro Yamanmoto, and Takaaki Yokozawa. Improving the absolute accuracy of the gravitational wave detectors by combining the photon pressure and gravity field calibrators. *Phys. Rev. D*, 98:022005, Jul 2018. doi: 10.1103/PhysRevD.98.022005. URL <https://link.aps.org/doi/10.1103/PhysRevD.98.022005>.
- [19] Michael P. Ross, Timesh Mistry, Laurence Datrier, Jeff Kissel, Krishna Venkateswara, Colin Weller, Kavic Kumar, Charlie Hagedorn, Eric Adelberger, John Lee, Erik Shaw, Patrick Thomas, David Barker, Filiberto Clara, Bubba Gateley, Tyler M. Guidry, Ed Daw, Martin Hendry, and Jens Gundlach. Initial results from the ligo newtonian calibrator. *Phys. Rev. D*, 104:082006, Oct 2021. doi:10.1103/PhysRevD.104.082006. URL <https://link.aps.org/doi/10.1103/PhysRevD.104.082006>.
- [20] Charles A. Hagedorn. *A Sub-Millimeter Parallel-Plate Test of Gravity*. PhD thesis, University of Washington, January 2015.
- [21] C Hagedorn and JG Lee. Newt (newtonian eot-wash toolkit). *GitHub*, 2021. URL <https://github.com/4kbt/NewtonianEotWashToolkit>.