8.4.3.1   Internal Adjustments Settings
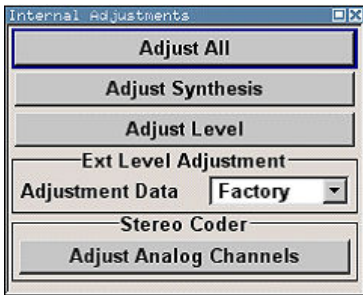
Access:

1. Press the [setup] key.

2. Select "System > Internal Adjustments".

In this dialog, you can perform internal calibration routines.

The remote commands required to define these settings are described in Chapter 6.4, "CALibration Subsystem", on page 290.

Settings

Adjust All

Performs all available internal calibration routines of the instrument.

Adjustment may take some time. Especially in instruments with frequencies above 6 GHz, it may last up to 15 minutes.

Remote command:
:CALibration:ALL[:MEASure]? on page 290

Adjust Synthesis

Performs all adjustments which affect the frequency.

Remote command:
:CALibration<hw>:FREQuency[:MEASure]? on page 291

Adjust Level

Performs all adjustments which affect the level. The acquired correction values improve the settling time and the signal quality.

Remote command:
:CALibration<hw>:LEVel[:MEASure]? on page 291