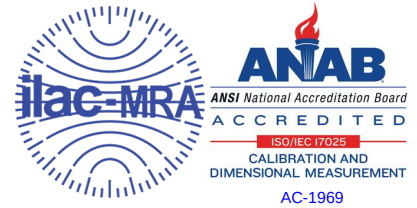




MICRO PRECISION CALIBRATION, INC
2165 N. Glassell St.,
Orange, CA 92865
714-901-5659



Certificate of Calibration

Date: Oct 4, 2022

Cert No. 551220085379184

Customer:

SILQ TECHNOLOGIES CORPORATION
607 CHARLES E YOUNG DR E
LOS ANGELES CA 90095

MPC Control #: LAF5769
Asset ID: LAF5769
Gage Type: ANALYTICAL BALANCE
Manufacturer: METTLER TOLEDO
Model Number: AB54-S
Size: 51 g
Temp/RH: 21.0°C / 43.0%
Location: Calibration performed at MPC facility

Work Order #: LA-90057418
Purchase Order #: CC
Serial Number: 1125311515
Department: N/A
Performed By: JOSE ACEVES
Received Condition: IN TOLERANCE
Returned Condition: IN TOLERANCE
Cal. Date: October 03, 2022
Cal. Interval: 12 MONTHS
Cal. Due Date: October 03, 2023

Calibration Notes:

See attached datasheet (2 pages)


Standards Used to Calibrate Equipment

I.D.	Description.	Model	Serial	Manufacturer	Cal. Due Date	Traceability #
LAS0092	Weight set 28 pc	CLASS E2	N/A	FUYUE	Apr 30, 2023	551220085343503


Procedures Used in this Event

Procedure Name	Description
MPC-WEI-001 Rev. 07	Weighing Instruments, General, rev.07, Jul-07-2021

Calibrating Technician:


JOSE ACEVES

QC Approval:


Gary Crouse

STATEMENTS OF PASS OR FAIL CONFORMANCE: The uncertainty of measurement has been taken into account when determining compliance with specification. All measurements and test results guard banded to ensure the probability of false-accept does not exceed 2% in compliance with ANSI/NCSL Z540.3-2006.

THE CALIBRATION REPORT STATUS:

PASS: Term used when compliance statement is given, and the measurement result is PASS.

PASS²: Term used when compliance statement is given, and the measurement result is conditional passed or PASS².

FAIL: Term used when compliance statement is given, and the measurement result is FAIL.

FAIL²: Term used when compliance statement is given, and the measurement result is conditional failed or FAIL².

REPORT OF VALUE: Term used when reported measurement is not requiring compliance statement in report.

ADJUSTED: When adjustments are made to an instrument which changes the value of measurement from what was measured as found to new value as left.

LIMITED: When an instrument fails calibration but is still functional in a limited manner.

The expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%, unless otherwise stated. This calibration report complies with ISO/IEC 17025:2017, ANSI/NCSL Z540.3-2006 and ANSI/NCSL Z540.1-1994. Calibration cycles and resulting due dates were submitted/approved by the customer. Any number of factors may cause an instrument to drift out of tolerance before the next scheduled calibration. Recalibration cycles should be based on frequency of use, environmental conditions and customer's established systematic accuracy. All standards are traceable to SI through the National Institute of Standards and Technology (NIST) and/or recognized national or international standards laboratories. Services rendered include proper manufacturer's service instruction and are warranted for no less than thirty (30) days. The information on this report pertains only to the instrument identified, this may not be reproduced in part or in a whole without the prior written approval of the issuing MP Calibration Laboratory.