

Calibration Report of Mettler Toledo AB54-S Analytical Balance

MPC Control #:	LAF5769	Serial Number:	1125311515
Asset ID:	LAF5769	Calibration Date:	October 03, 2022

Repeatability

Range	Applied	Lower Limit	As Found	As Left	Upper Limit	Result	Uncertainty ($\pm$)	TUR
51.0000 g	20.0000 g	19.9998 g	20.0001 g	20.0001 g	20.0002 g	PASS	0.000089 g	2.2 : 1

The standard deviation was found to be 0.000 g


Linearity

Range	Applied	Lower Limit	As Found	As Left	Upper Limit	Result	Uncertainty ($\pm$)	TUR
51.0000 g	5.0000 g	4.9996 g	5.0002 g	5.0002 g	5.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$
51.0000 g	12.0000 g	11.9996 g	12.0000 g	12.0000 g	12.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$
51.0000 g	25.0000 g	24.9996 g	25.0001 g	25.0001 g	25.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$
51.0000 g	38.0000 g	37.9996 g	38.0003 g	38.0003 g	38.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$
51.0000 g	51.0000 g	50.9996 g	51.0003 g	51.0003 g	51.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$

Eccentricity

Position	Applied	Lower Limit	As Found	Deviation from Center	Upper Limit	Result	Uncertainty ($\pm$)	TUR
Center (1)	20.0000 g	19.9996 g	20.0001 g	0.0000 g	20.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$
Front Left (2)	20.0000 g	19.9996 g	20.0001 g	0.0000 g	20.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$
Back Left (3)	20.0000 g	19.9996 g	20.0002 g	0.0001 g	20.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$
Back Right (4)	20.0000 g	19.9996 g	20.0000 g	0.0001 g	20.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$
Front Right (5)	20.0000 g	19.9996 g	20.0001 g	0.0000 g	20.0004 g	PASS	0.000089 g	$\geq 4.0 : 1$

Platform Eccentricity Loading Positions



Max Deviation from Center	Position(s)
0.0001 g	(3) (4)

Calibration Report of Mettler Toledo AB54-S Analytical Balance

MPC Control #: LAF5769
Asset ID: LAF5769

Serial Number: 1125311515
Calibration Date: October 03, 2022


Statements of Pass or Fail Conformance

The uncertainty of measurement has been taken into account when determining compliance with specification.

All measurements and test results guard banded to ensure the probability of false-accept does not exceed 2% in compliance with ANSI/NCSL Z540.3-2006

The status of compliance with the acceptance criteria is reported as:

- PASS** — Compliant with specification.
- PASS^z** — The measured value is within acceptance limits.
However, a portion of the expanded uncertainty of measurement at 95% exceeds the specified tolerance.
- FAIL^z** — The measured value is not within the acceptance limits.
However, a portion of the expanded uncertainty of measurement at 95% is within the specified tolerance.
- FAIL** — Not compliant with specification.

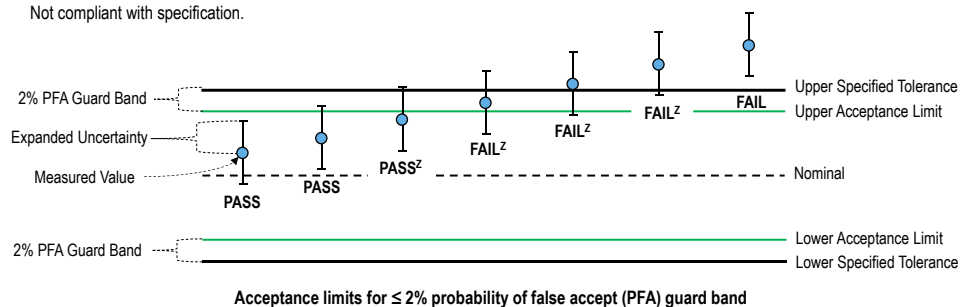

The expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95%, unless otherwise stated.

This calibration report complies with ISO/IEC 17025:2017 and ANSI/NCSL Z540.3-2006, Method 6 --- Guard Bands Based on Test Uncertainty Ratio.

- End of Calibration Report -