


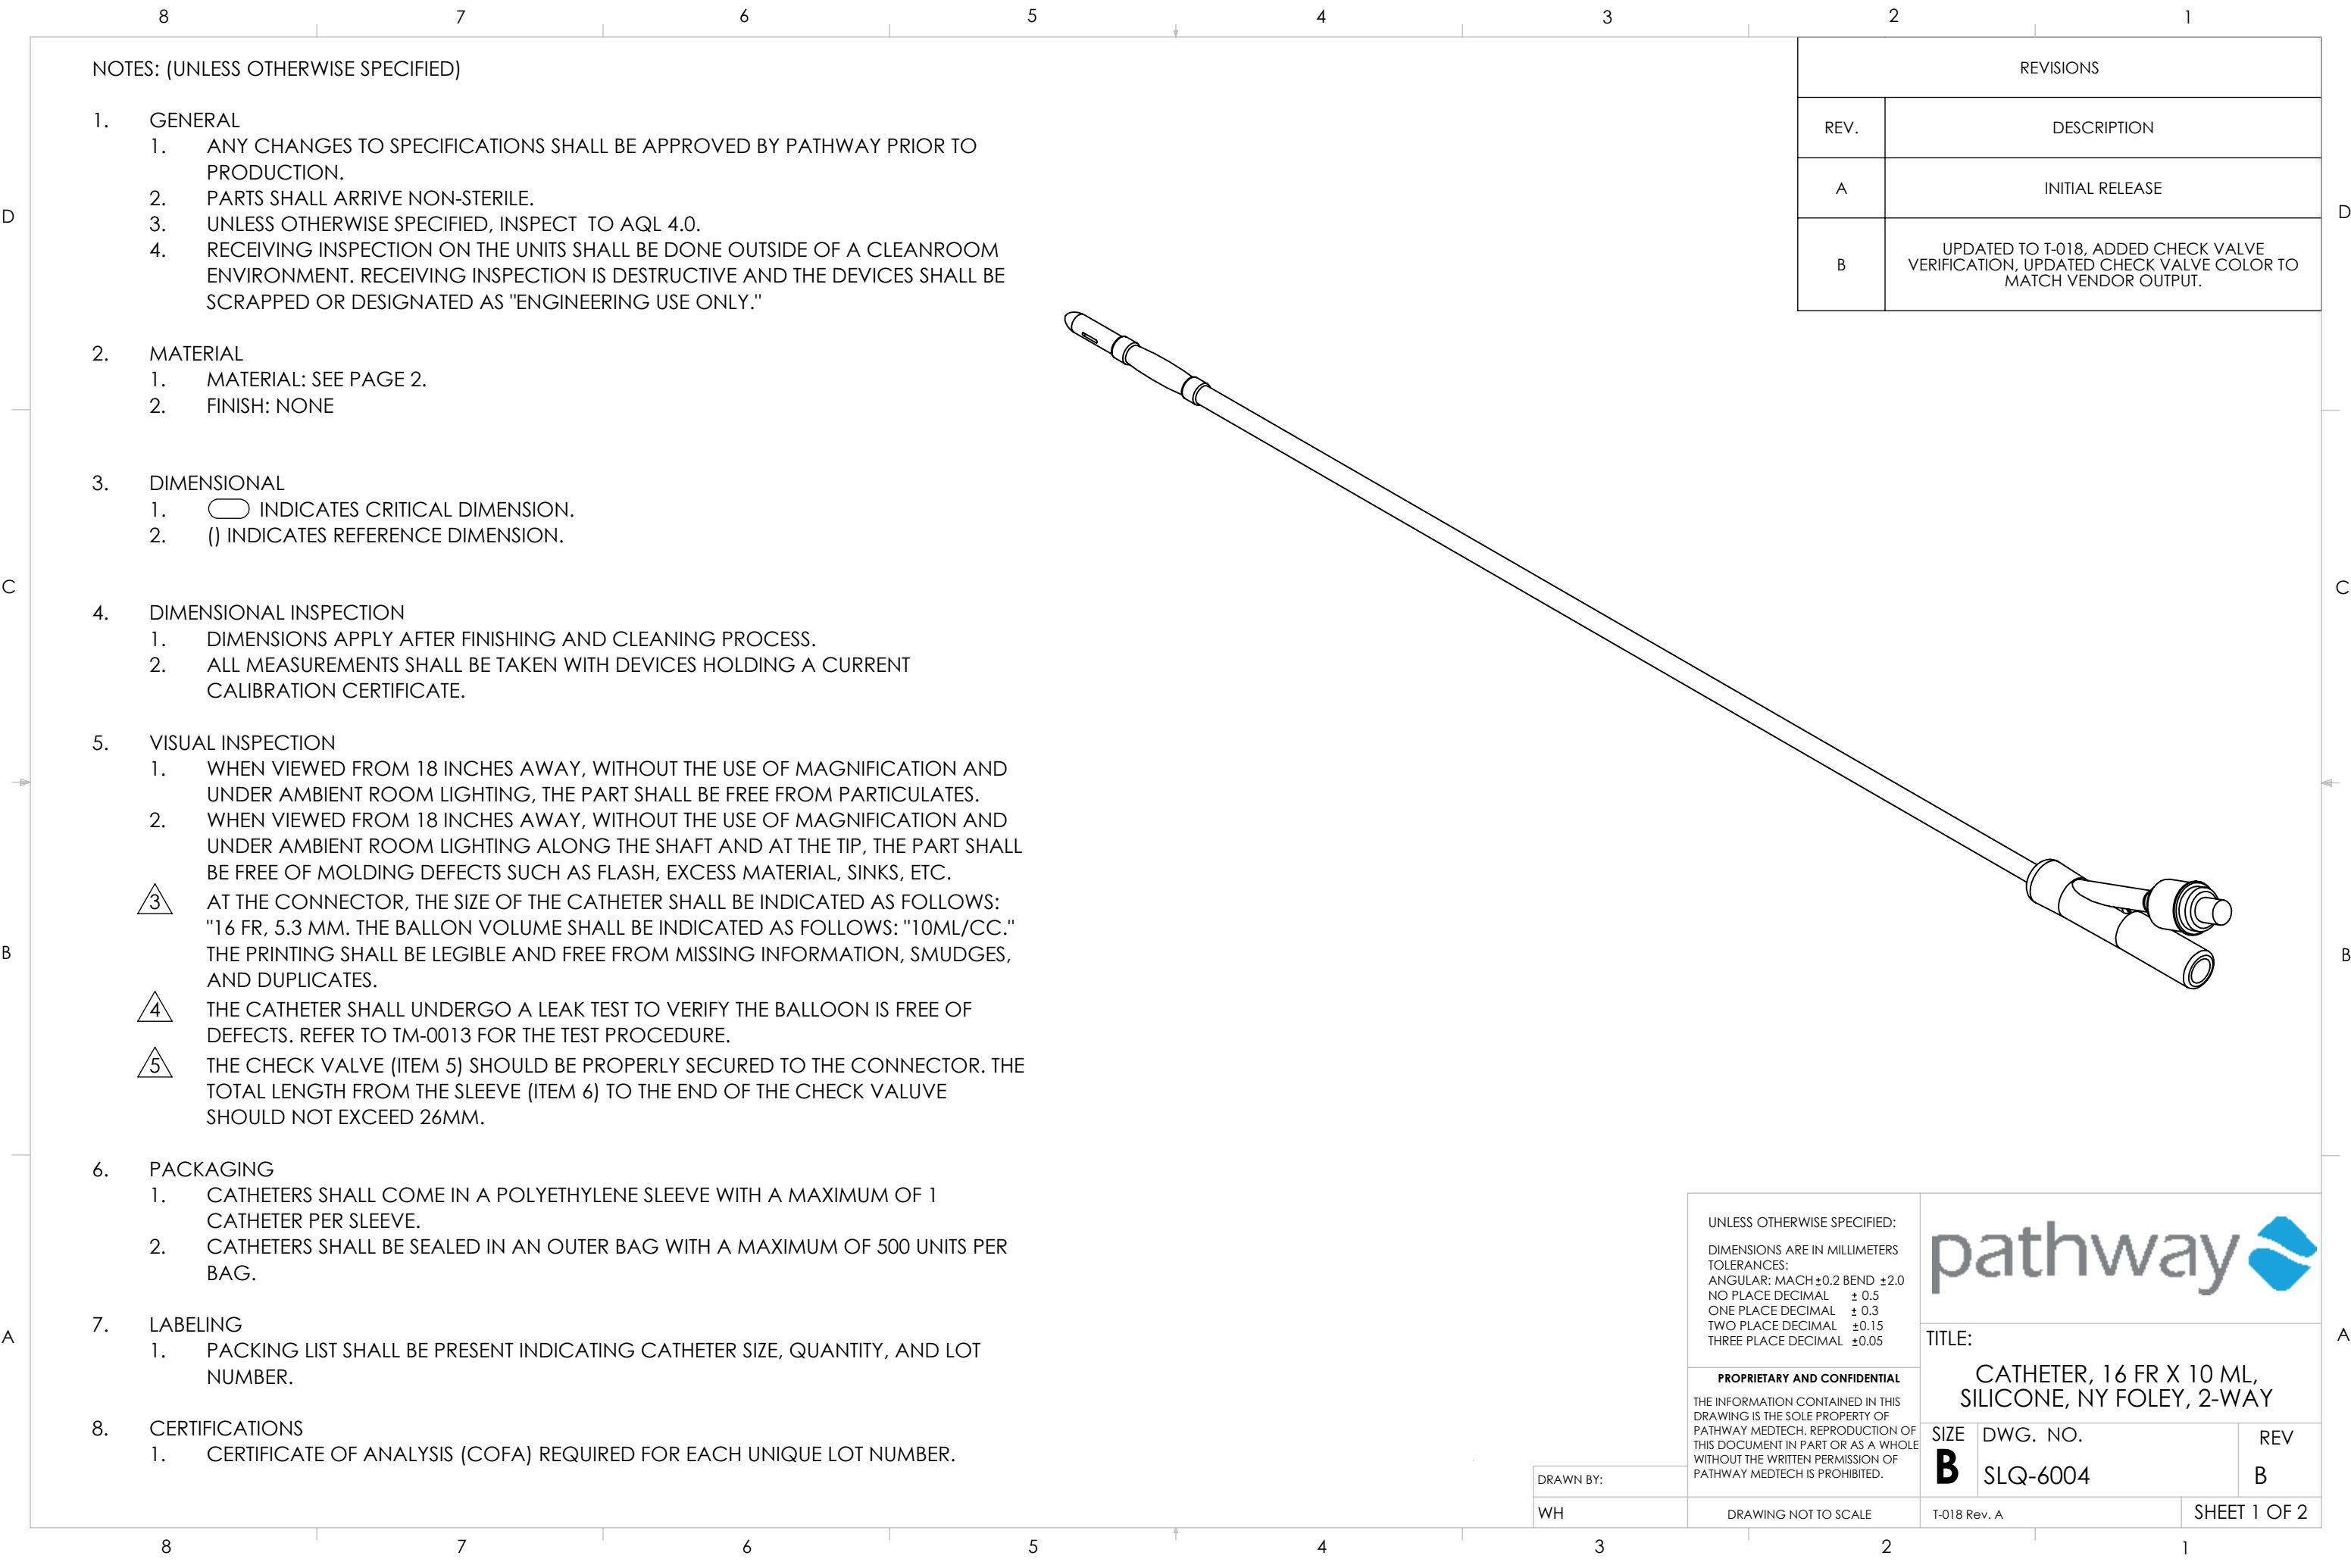

NOTES: (UNLESS OTHERWISE SPECIFIED)

1. GENERAL

- 1. ANY CHANGES TO SPECIFICATIONS SHALL BE APPROVED BY PATHWAY PRIOR TO PRODUCTION.
- 2. PARTS SHALL ARRIVE NON-STERILE.
- 3. UNLESS OTHERWISE SPECIFIED, INSPECT TO AQL 4.0.
- 4. RECEIVING INSPECTION ON THE UNITS SHALL BE DONE OUTSIDE OF A CLEANROOM ENVIRONMENT. RECEIVING INSPECTION IS DESTRUCTIVE AND THE DEVICES SHALL BE SCRAPPED OR DESIGNATED AS "ENGINEERING USE ONLY."

2. MATERIAL

- 1. MATERIAL: SEE PAGE 2.
- 2. FINISH: NONE

3. DIMENSIONAL

- 1.  INDICATES CRITICAL DIMENSION.
- 2. () INDICATES REFERENCE DIMENSION.

4. DIMENSIONAL INSPECTION

- 1. DIMENSIONS APPLY AFTER FINISHING AND CLEANING PROCESS.
- 2. ALL MEASUREMENTS SHALL BE TAKEN WITH DEVICES HOLDING A CURRENT CALIBRATION CERTIFICATE.

5. VISUAL INSPECTION

- 1. WHEN VIEWED FROM 18 INCHES AWAY, WITHOUT THE USE OF MAGNIFICATION AND UNDER AMBIENT ROOM LIGHTING, THE PART SHALL BE FREE FROM PARTICULATES.
- 2. WHEN VIEWED FROM 18 INCHES AWAY, WITHOUT THE USE OF MAGNIFICATION AND UNDER AMBIENT ROOM LIGHTING ALONG THE SHAFT AND AT THE TIP, THE PART SHALL BE FREE OF MOLDING DEFECTS SUCH AS FLASH, EXCESS MATERIAL, SINKS, ETC.

 AT THE CONNECTOR, THE SIZE OF THE CATHETER SHALL BE INDICATED AS FOLLOWS: "16 FR, 5.3 MM. THE BALLON VOLUME SHALL BE INDICATED AS FOLLOWS: "10ML/CC." THE PRINTING SHALL BE LEGIBLE AND FREE FROM MISSING INFORMATION, SMUDGES, AND DUPLICATES.

 THE CATHETER SHALL UNDERGO A LEAK TEST TO VERIFY THE BALLOON IS FREE OF DEFECTS. REFER TO TM-0013 FOR THE TEST PROCEDURE.

 THE CHECK VALVE (ITEM 5) SHOULD BE PROPERLY SECURED TO THE CONNECTOR. THE TOTAL LENGTH FROM THE SLEEVE (ITEM 6) TO THE END OF THE CHECK VALUVE SHOULD NOT EXCEED 26MM.

6. PACKAGING

- 1. CATHETERS SHALL COME IN A POLYETHYLENE SLEEVE WITH A MAXIMUM OF 1 CATHETER PER SLEEVE.
- 2. CATHETERS SHALL BE SEALED IN AN OUTER BAG WITH A MAXIMUM OF 500 UNITS PER BAG.

7. LABELING

- 1. PACKING LIST SHALL BE PRESENT INDICATING CATHETER SIZE, QUANTITY, AND LOT NUMBER.

8. CERTIFICATIONS

- 1. CERTIFICATE OF ANALYSIS (COFA) REQUIRED FOR EACH UNIQUE LOT NUMBER.

REVISIONS	
REV.	DESCRIPTION
A	INITIAL RELEASE
B	UPDATED TO T-018, ADDED CHECK VALVE VERIFICATION, UPDATED CHECK VALVE COLOR TO MATCH VENDOR OUTPUT.

UNLESS OTHERWISE SPECIFIED:
DIMENSIONS ARE IN MILLIMETERS
TOLERANCES:
ANGULAR: MACH $\pm$ 0.2 BEND $\pm$ 2.0
NO PLACE DECIMAL $\pm$ 0.5
ONE PLACE DECIMAL $\pm$ 0.3
TWO PLACE DECIMAL $\pm$ 0.15
THREE PLACE DECIMAL $\pm$ 0.05

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF PATHWAY MEDTECH. REPRODUCTION OF THIS DOCUMENT IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF PATHWAY MEDTECH IS PROHIBITED.



TITLE:
CATHETER, 16 FR X 10 ML,
SILICONE, NY FOLEY, 2-WAY

DRAWN BY:		SIZE	DWG. NO.	REV
WH	DRAWING NOT TO SCALE	B	SLQ-6004	B
T-018 Rev. A		SHEET 1 OF 2		

ITEM NO.	DESCRIPTION	MATERIAL	COLOR	QTY.	NOTES
1	SHAFT	SILICONE YM827	NATURAL	1	BLUE STRIPE DEVELOPED UNDER X-RAY AND CONTAINS BARIUM SULFATE
2	BALLOON	SILICONE YM827	NATURAL	1	ORDINARY BALLOON TYPE
3	TIP	SILICONE YM827	BLUE	1	DEVELOPED UNDER X-RAY, CONTAINS BARIUM SULFATE
4	FUNNEL	SILICONE YM827	NATURAL	1	N/A
5	CHECK VALVE	PP, PVC, ABS, SILICONE, AND STAINLESS STEEL	TRANSPARENT / BLUE	1	BESPAK MED
6	SLEEVE	PP	ORANGE	1	N/A

D

C

B

A

E




E

D


C

B

A

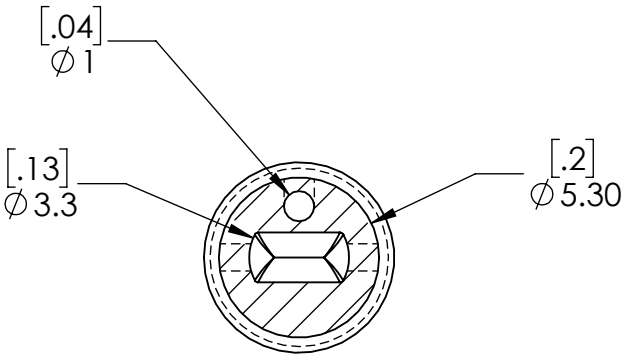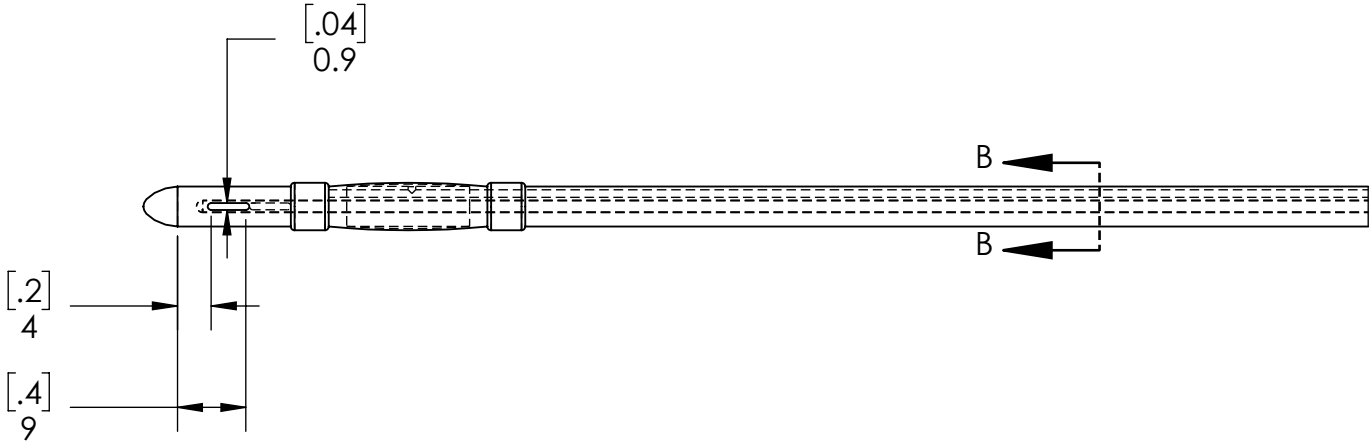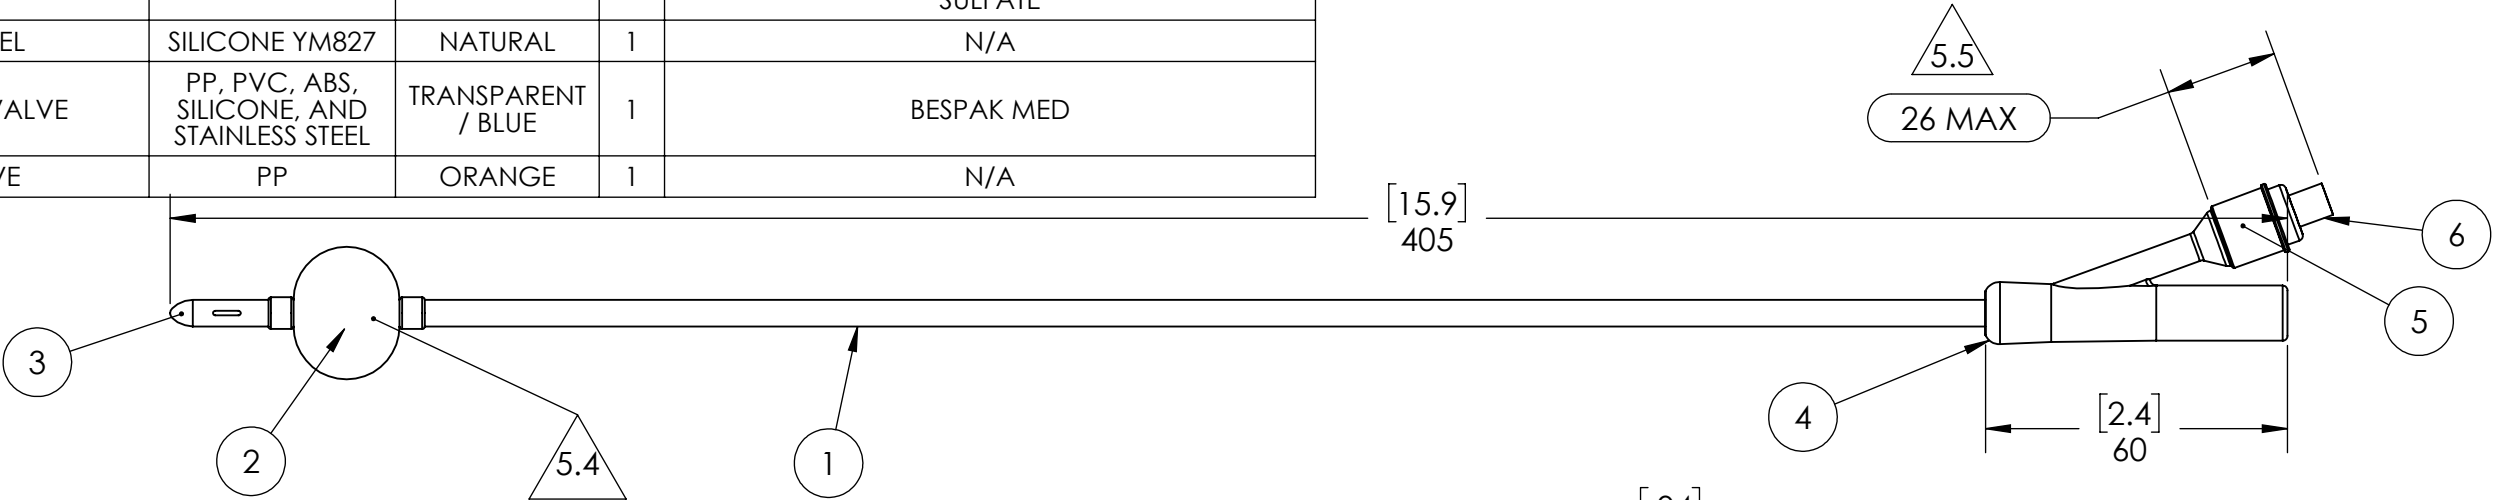

SECTION B-B
SCALE 4 : 1

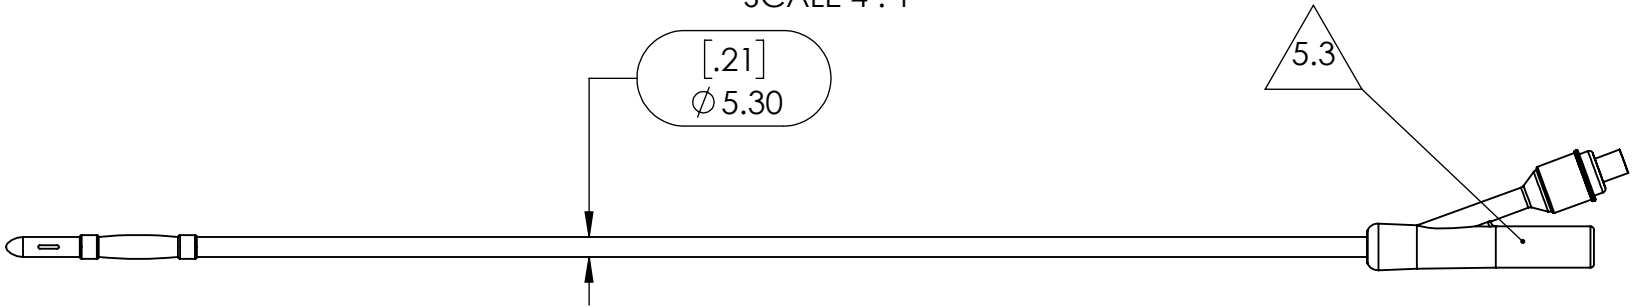

SIZE	DWG. NO.	REV
B	SLQ-6004	B
T-018 Rev. A	SHEET 2 OF 2	