



DOCUMENT TITLE:
Suspension Quality Control Report

Revision:
A

DOCUMENT #:
TMP1-QC-C.SLQ001

Effective Date:
23Sep2022

General Production Information

Work Order #:	2209-01	NCMR #:	N/A
Part Number:	C.SLQ001	Manufacture & Expiration Date:	Mfg date: 09-28-22 Exp date: 09-28-23
Part Revision:	B	Batch / Lot #:	2209-01-1

Supplies Traceability

Part Number	Description	Part Revision	Lot / Batch #
S.SLQ005	pH Strip	A	10BDH4801
S.SLQ006	Deuterium oxide	A	M2338

Equipment Traceability

Part Number	Description	Equipment ID	Calibration Due Date
E.SLQ013	Weighing scale	ST-012	10/3/23

QC Data

Sample Tube	Weight Empty (g)	Weight with Residue (g)	Residue Net Weight (g)
Sample A1	13.122	13.2269	.1049
Sample A2	13.0385	13.1439	.1054
Sample B1	13.0422	13.1407	0.0985
Sample B2	13.1333	13.2355	.1022
Sample C1	13.0062	13.1099	0.1037
Sample C2	13.1458	13.2462	.1004

	DOCUMENT TITLE: Suspension Quality Control Report	Revision: A
	DOCUMENT #: TMP1-QC-C.SLQ001	Effective Date: 23Sep2022

Sample Tube	Weight Empty (g)	Weight with Sample suspended (g)	Weight with Residue on Evaporation (g)	Residue on Evaporation (%)
Suspension Test Sample	13.1365	43.2069		
Residue on Evaporation Sample	13.1353	23.2289	13.2383	1.030%

Summary of Results

Attribute	Result	Acceptance criteria	Meets Criteria? (circle one)
Appearance (color)	Opaque white	Opaque white	☒ Yes No
Appearance (form)	Inviscid liquid	Inviscid liquid	☒ Yes No
Residue on Evaporation	1.030%	0.5% – 1.5%	☒ Yes No
pH	6.0	5 – 8	☒ Yes No
¹ H NMR	Attach ¹ H NMR spectra	Identify Peaks with Amplitude >5% of Solvent Peak (4.75ppm)	☒ Yes No
¹⁹ F NMR	Attach ¹⁹ F NMR spectra	Identify Peaks, if there is a peak at -76ppm determine approximate amplitude relative to peaks at -140ppm and -150ppm	☒ Yes No

Report completed by:

<u>Ethan Rao</u>	<u>Ethan Rao</u>	<u>09-Nov-2022</u>
Print name	Signature	Date

Report reviewed by:

<u>Bryan Wong</u>	<u>Bryan Wong</u>	<u>09 Nov 2022</u>
Print name	Signature	Date



DOCUMENT TITLE:
Suspension Quality Control Report


Revision:
A

DOCUMENT #:
TMP1-QC-C.SLQ001

Effective Date:
23Sep2022


¹H NMR:

2209-01-1

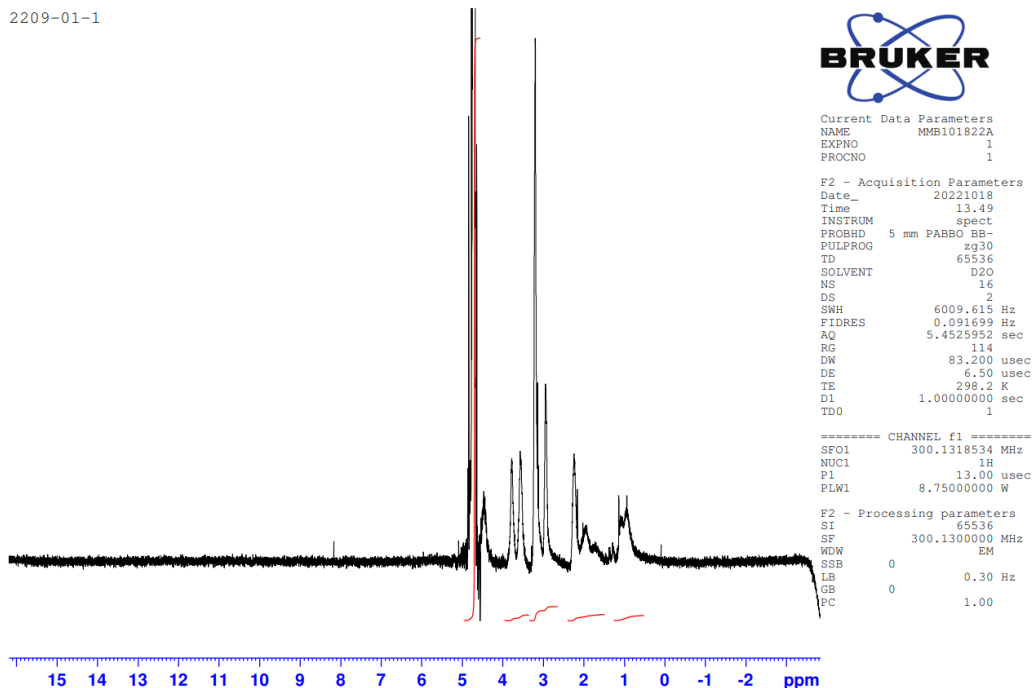

Broad Peaks are present at approximately 0.99, 2.2, 2.9, 3.1, 3.5, 3.7, 4.4, and 4.75 ppm indicating successful incorporation of the zwitterion moiety into the polymer.

¹⁹F NMR:

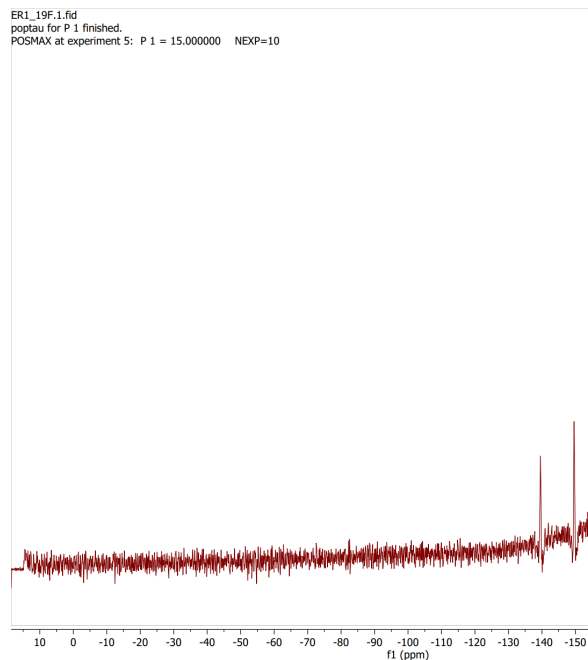

	DOCUMENT TITLE: Suspension Quality Control Report	Revision: A
	DOCUMENT #: TMP1-QC-C.SLQ001	Effective Date: 23Sep2022

Two peaks at -140 and -150 ppm identified. No peak was present at -76ppm indicating there is no TFE remaining in the suspension.