


## ClearTract™ 2-Way Foley Catheter

Surface treatment that creates  
a unique hydration layer


100% Medical  
Grade Silicone

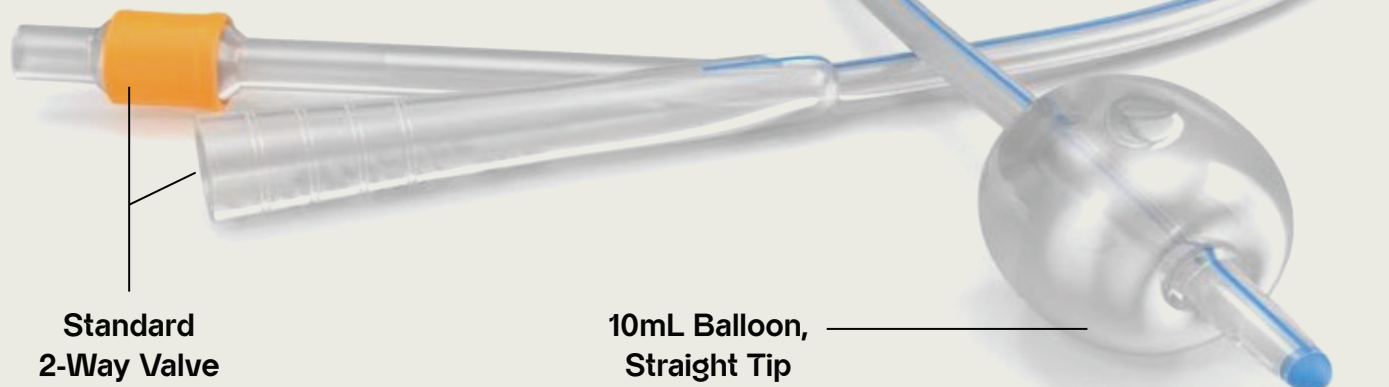


## Biofilm

Biofilms have been identified as a major cause of hospital-acquired infection. Microorganisms anchor to the surface of implantable devices and grow into resilient biofilms that become 1000x more resistant to antibiotics than in their non-biofilm state.

ACTIVE BIOMASS CONTENT\*  
\*AS INDICATED BY BACTITER-GLO ATPASE ASSAY

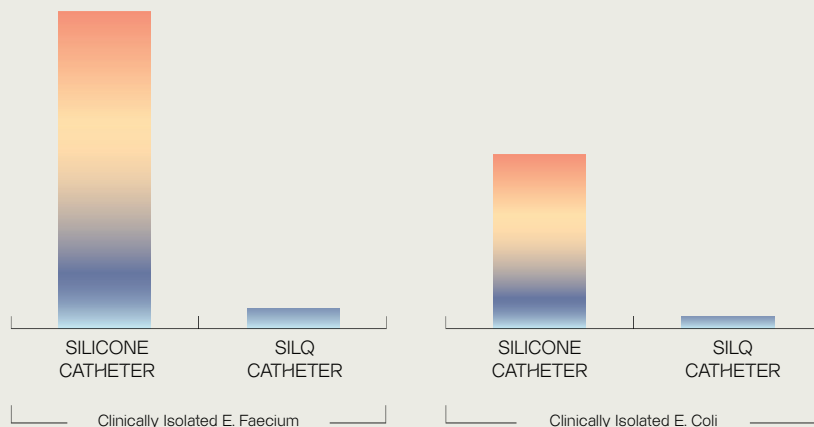

### SILICONE SURFACE

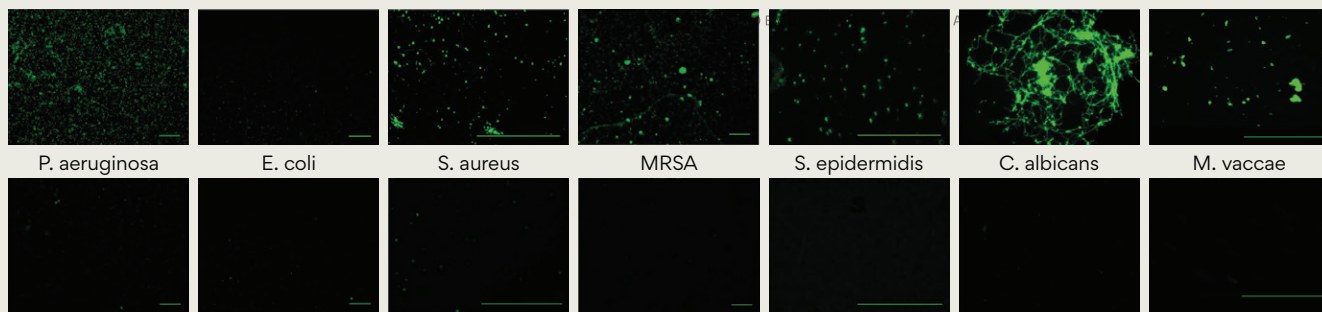

### SILICONE SURFACE WITH SILQ

# ClearTract™ Catheters

Made from 100% medical grade silicone

**NO LATEX**


**NO BPA**

**NO DEHP**

The days of latex healthcare products are coming to an end as 4.3% of the world population has a sensitivity to latex. Healthcare workers have more than double the sensitivity rate because latex sensitivity manifests from repeated exposure. Silicone is well-known for exceptional biocompatibility and has replaced latex in most applications. ClearTract™ Catheters are made from 100% medical grade silicone known for its exceptional biocompatibility, protecting both your patients and employees.


# Fibrinogen

Adhesion of fibrinogen and other proteins to surfaces plays a large role in the blood-clotting cascade.

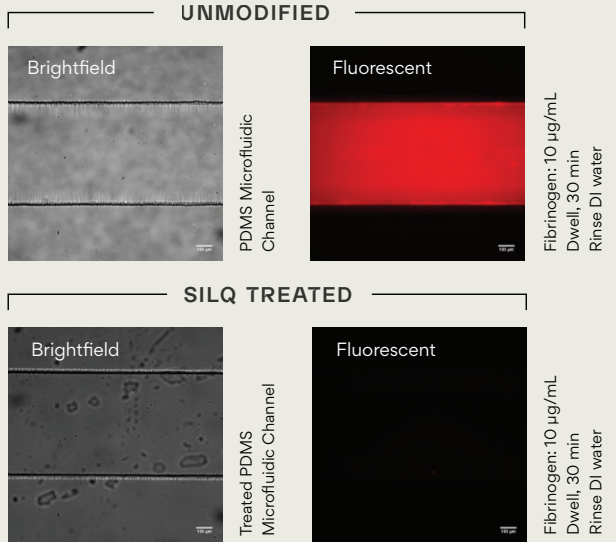

# Coefficient of Friction


SILQ formulation reduces the tackiness of silicone surface by 15X.

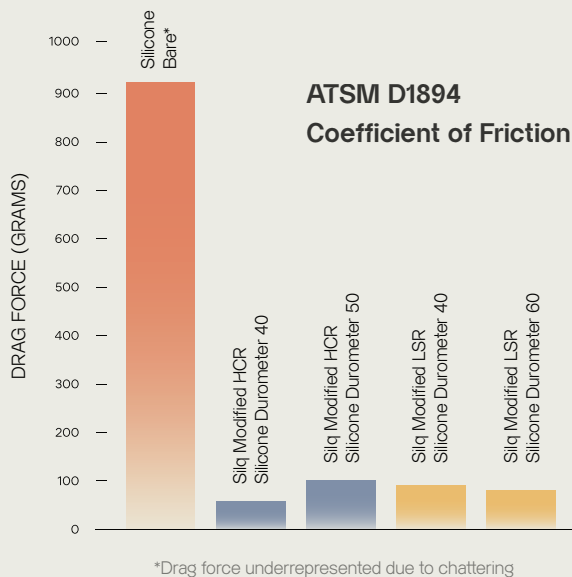

# Biocompatibility FDA Clearance

Silq-treated devices have been cleared by the FDA based on strict biocompatibility testing specifications listed in ISO 10993-18:2020:

- Cytotoxicity
- Systemic Toxicity
- Irritation
- Sensitization
- Sub-acute Toxicity
- Sub-chronic Toxicity

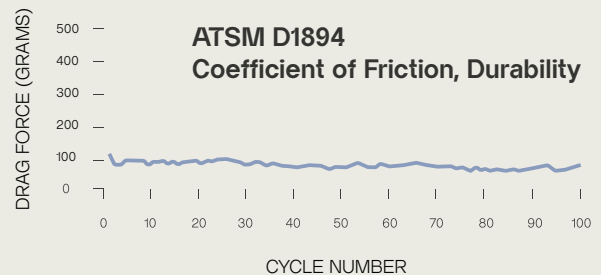

# ClearTract™ Foley Catheter - Ordering Information

| Catheter Size | Balloon Size | Valve | Catheter SKU# |
|---------------|--------------|-------|---------------|
| 14F           | 10cc         | 2-Way | 21400101003   |
| 16F           | 10cc         | 2-Way | 21600101003   |
| 18F           | 10cc         | 2-Way | 21800101003   |

\*All test data available on file