


DVF QA pipeline report

DIR-Lab-case5


Field	Value
Case	DIR-Lab-case5
Generated	2026-05-20 09:25:15
source	Case5Pack
fps	15.0
n_cycles	4
frames_per_cycle	30
n_phases	10
ct_shape	(106, 256, 256)
spacing_xyz_mm	(1.1, 1.1, 2.5)
detector_shape	(256, 256)
pixel_spacing_mm	(1.0, 1.0)
device	cpu

4DCT phase preview


ϕ_0

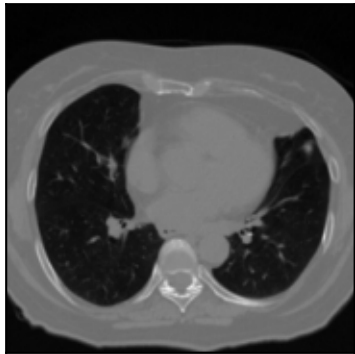


ϕ_1

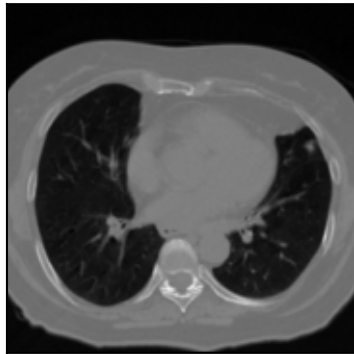


ϕ_2

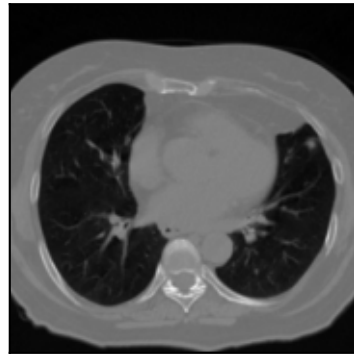

ϕ_3

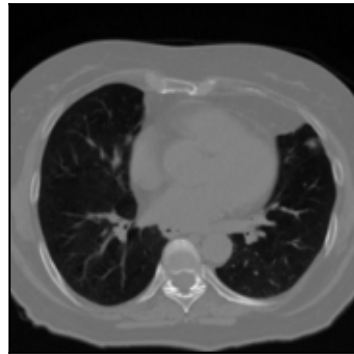

ϕ_4

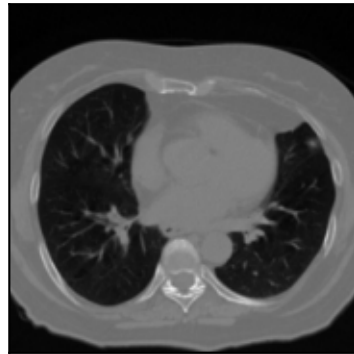


ϕ_5




ϕ_6




ϕ_7

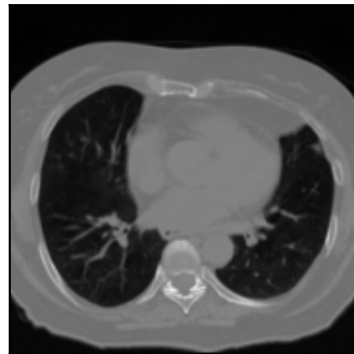

ϕ_8

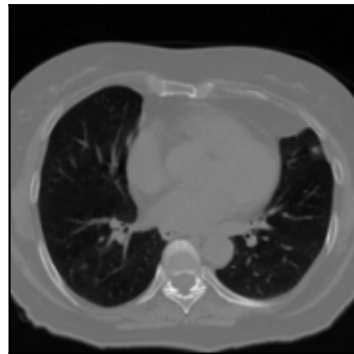

ϕ_9

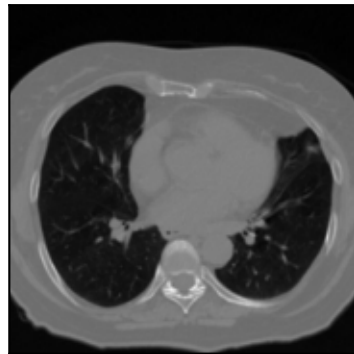

Per-phase DRRs

AP ϕ_0



AP ϕ_1



AP ϕ_2



AP ϕ_3



AP ϕ_4



AP ϕ_5



AP ϕ_6



AP ϕ_7



AP ϕ_8



AP ϕ_9



Lat ϕ_0



Lat ϕ_1



Lat ϕ_2



Lat ϕ_3



Lat ϕ_4



Lat ϕ_5



Lat ϕ_6



Lat ϕ_7



Lat ϕ_8



Lat ϕ_9



Dynamic sequence samples


AP t=0 (0.00s)




AP t=24 (1.60s)



AP t=48 (3.20s)

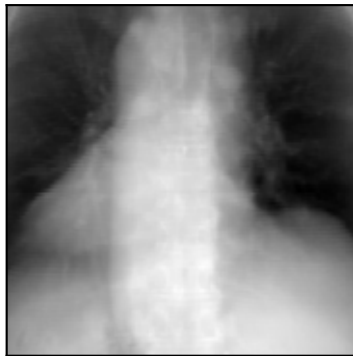

AP t=72 (4.80s)

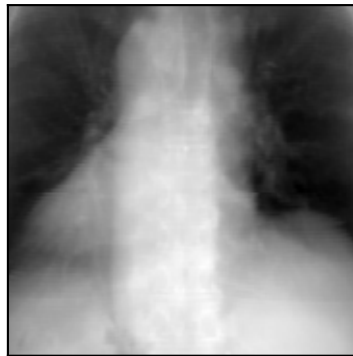

AP t=96 (6.40s)



AP t=120 (8.00s)




Lat t=0



Lat t=24



Lat t=48

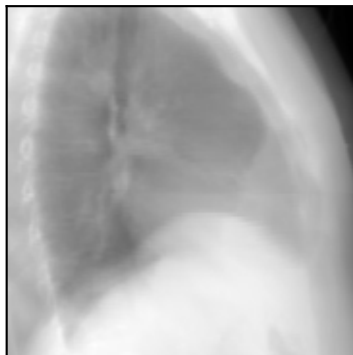

Lat t=72




Lat t=96



Lat t=120




Driving phase curve
Driving phase curve (ground-truth respiratory motion)

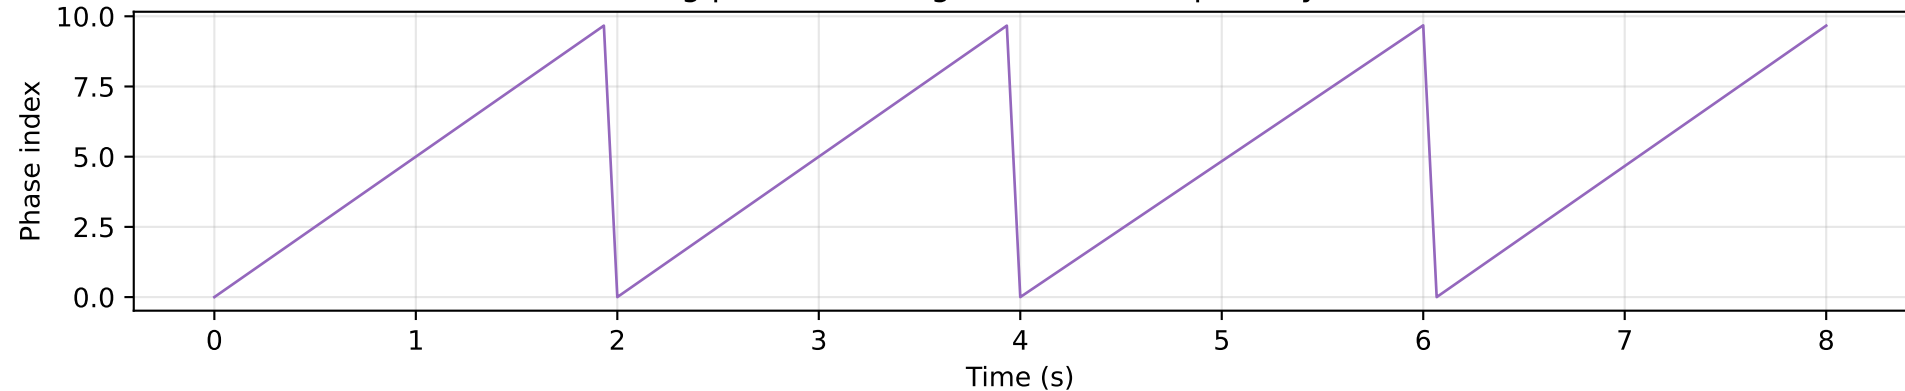


Amsterdam Shroud — AP

AP shroud + tracked diaphragm

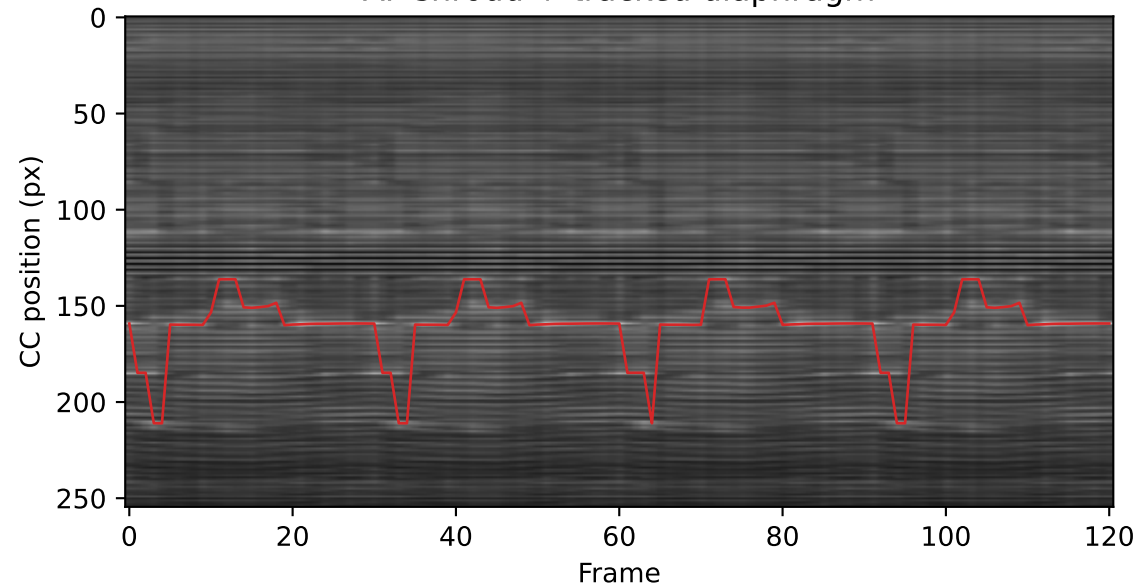


AP respiratory signal | $f=0.496$ Hz

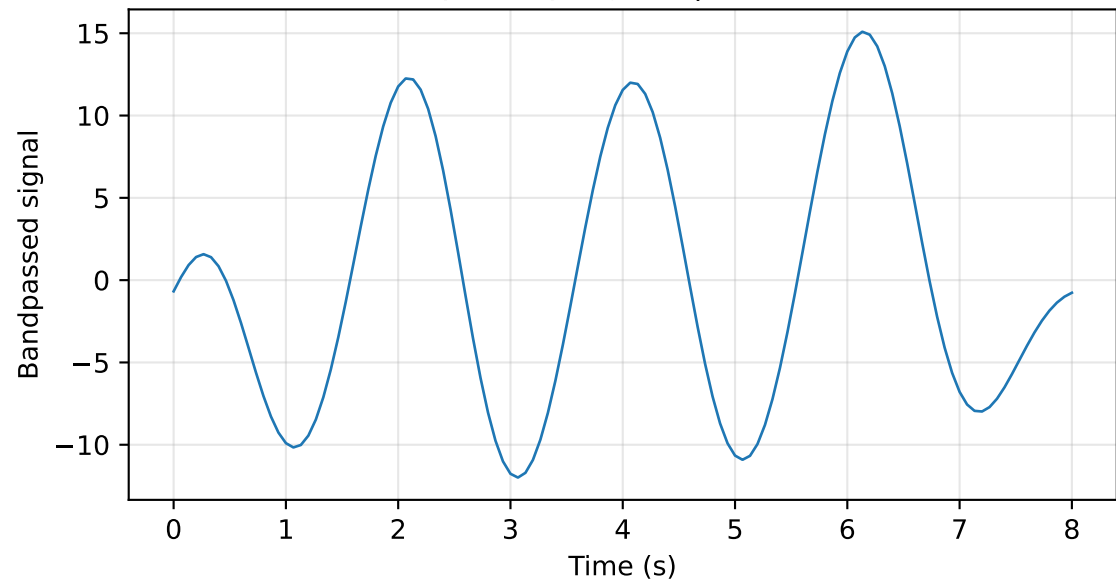


Amsterdam Shroud — Lateral

Lateral shroud + tracked diaphragm

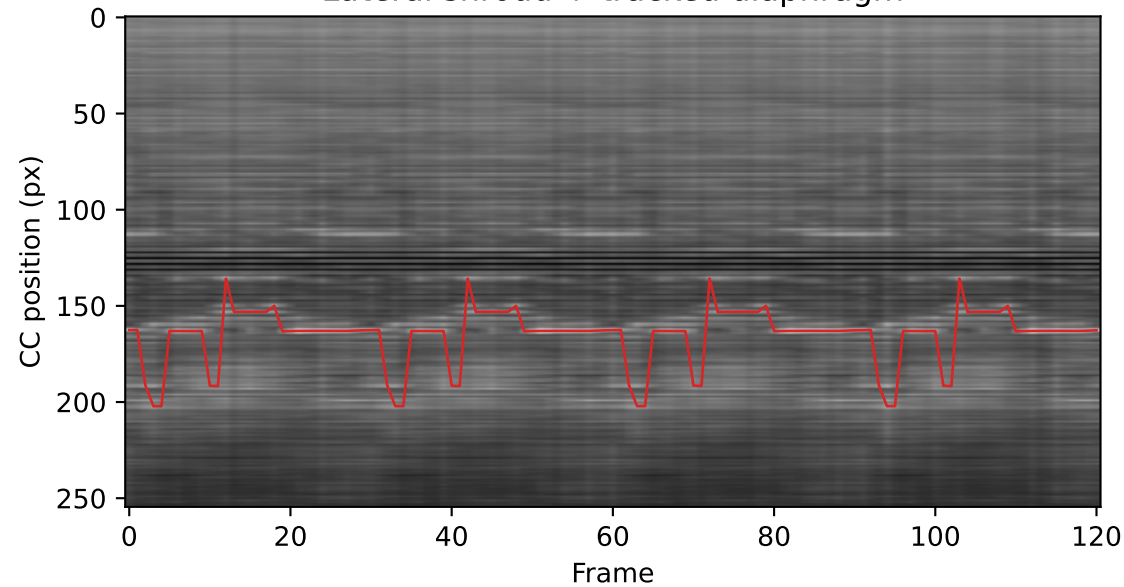


Lateral respiratory signal | $f=0.496$ Hz

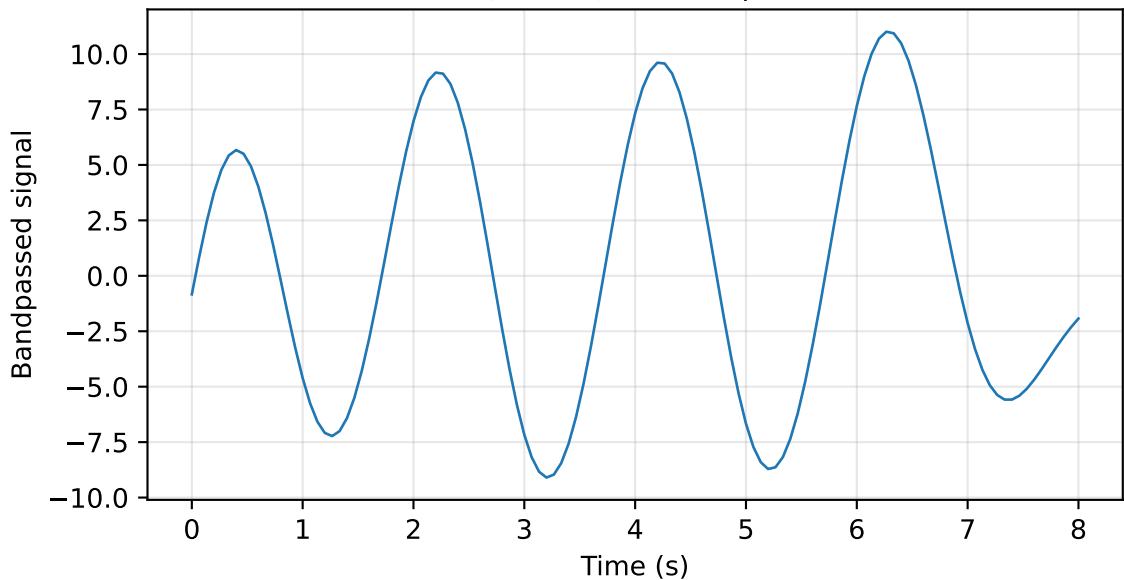


Cycle pairing


AP signal (selected cycle highlighted)

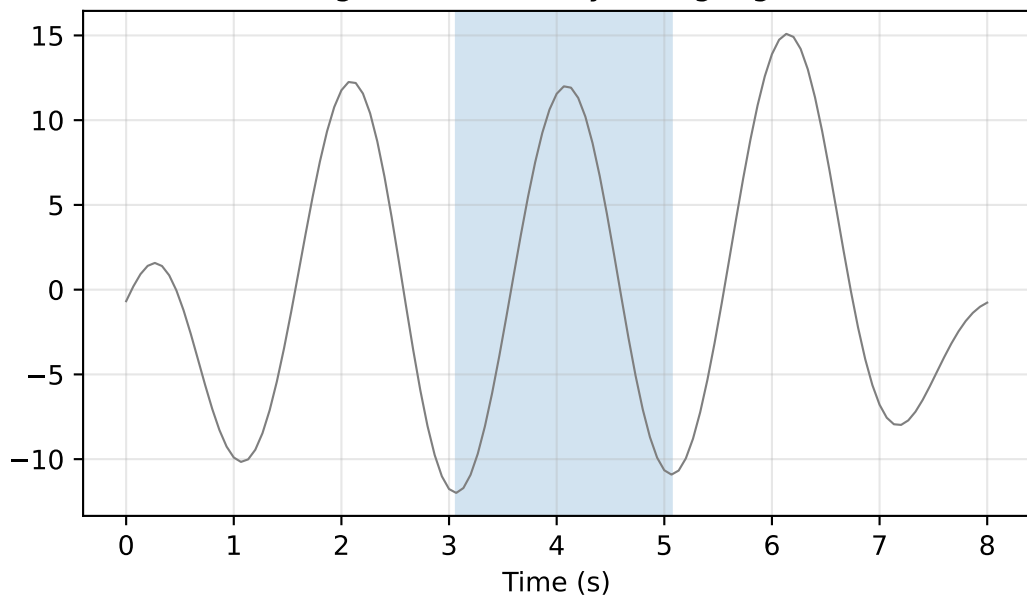


Lateral signal (selected cycle highlighted)

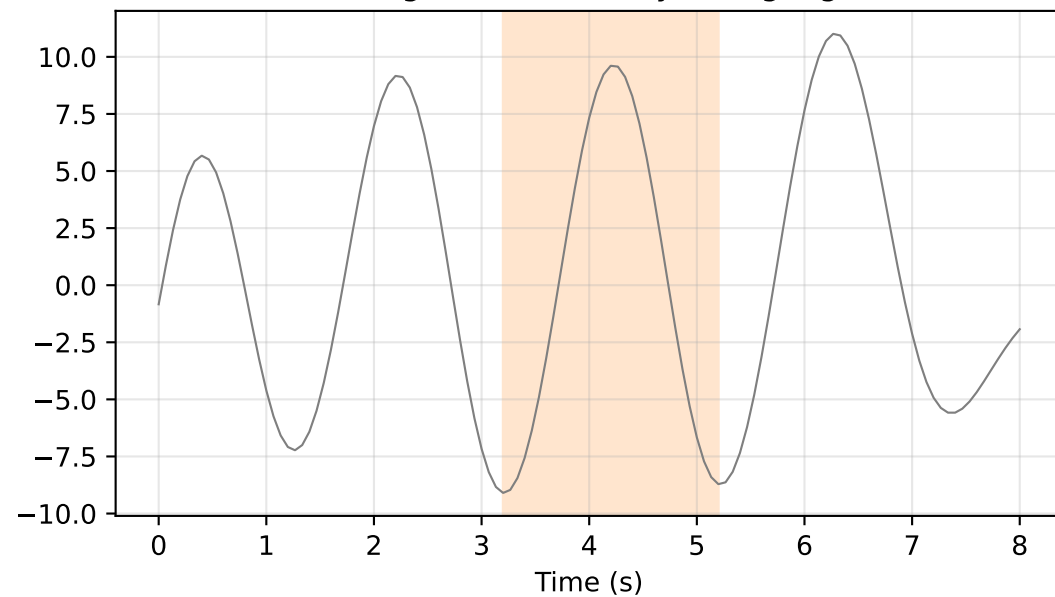

NCC matrix (best=1.000)

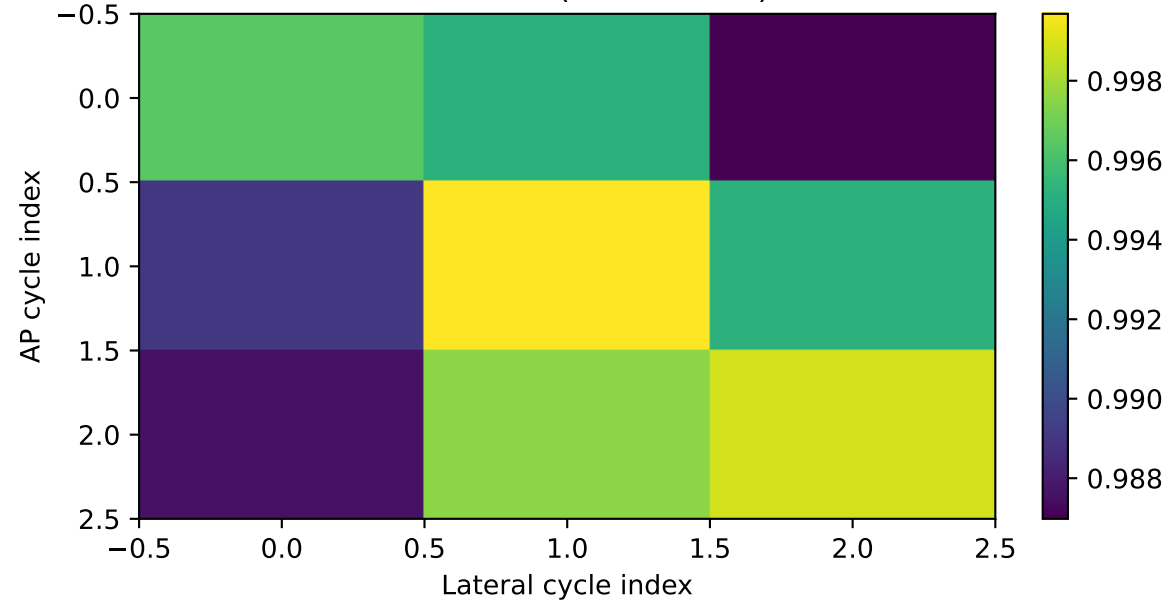

Selected cycle overlay

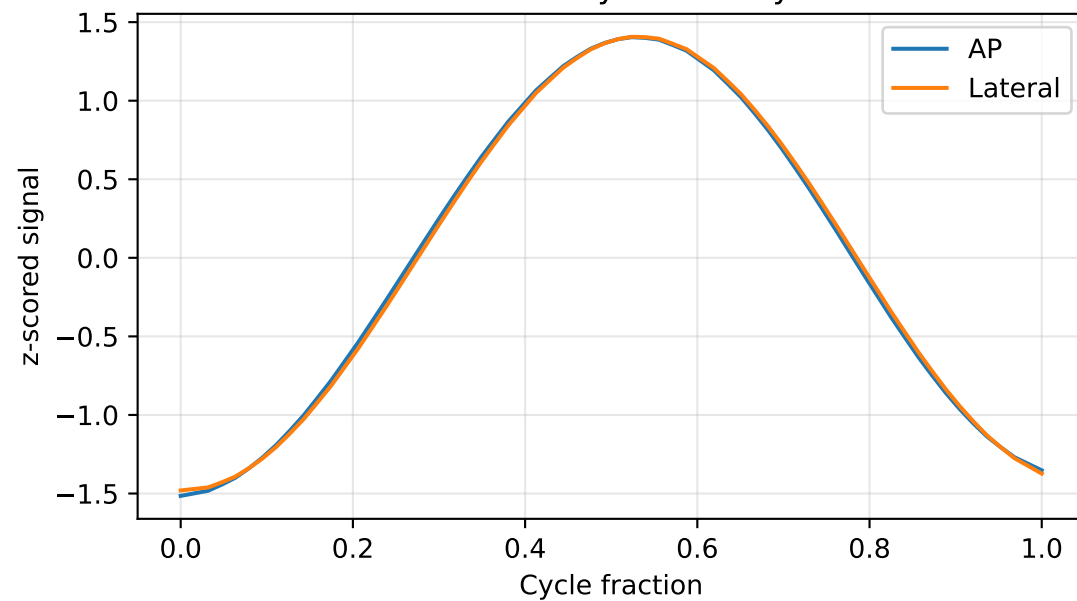

Metrics

Metric	Value
AP dominant frequency (Hz)	0.4959
AP period (frames)	30.25
Lateral dominant frequency (Hz)	0.4959
Lateral period (frames)	30.25
Best pair NCC	0.9997
AP cycle frames	46 - 76
Lateral cycle frames	48 - 78
min_period_s	1.0000