

Module status

phase 40 — Module status

Module	Status
TemporalMotion	FAIL
RobustnessCheck	FAIL
GeomIntegrity	FAIL
DosimetricAccuracy	ERROR




CT comparison

Synthetic (warped 50→PP)




Planning (phase 50)

|Synthetic – Planning|




Axial mid

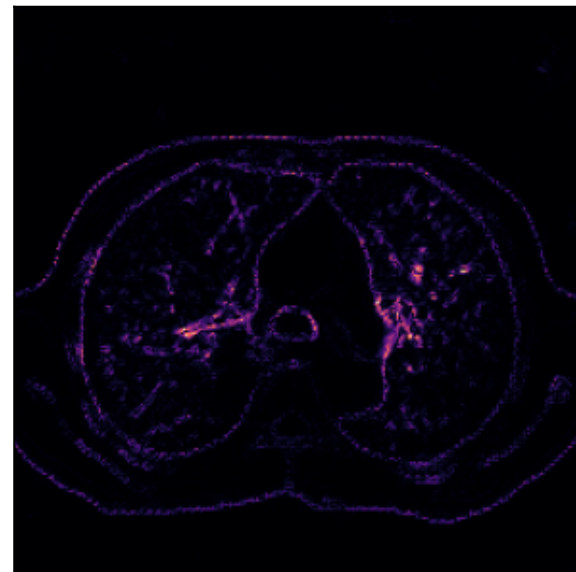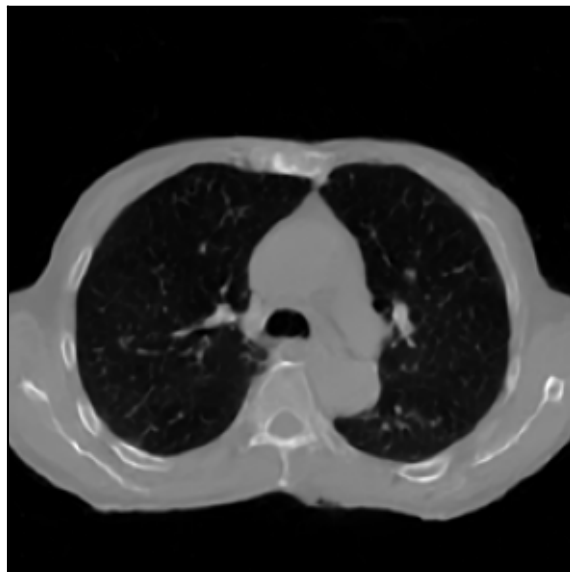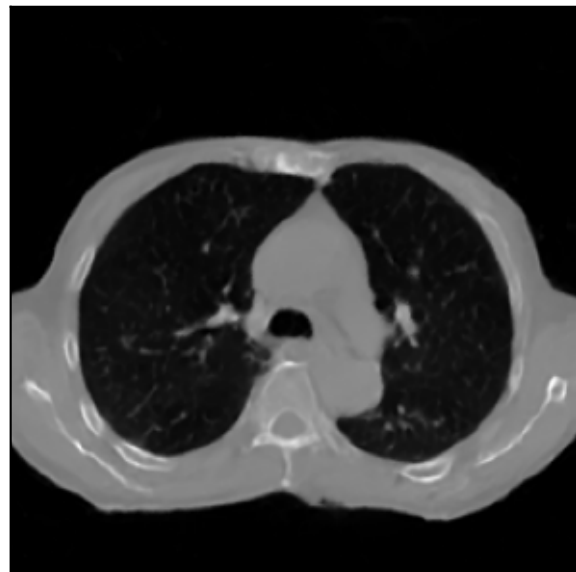

Coronal mid

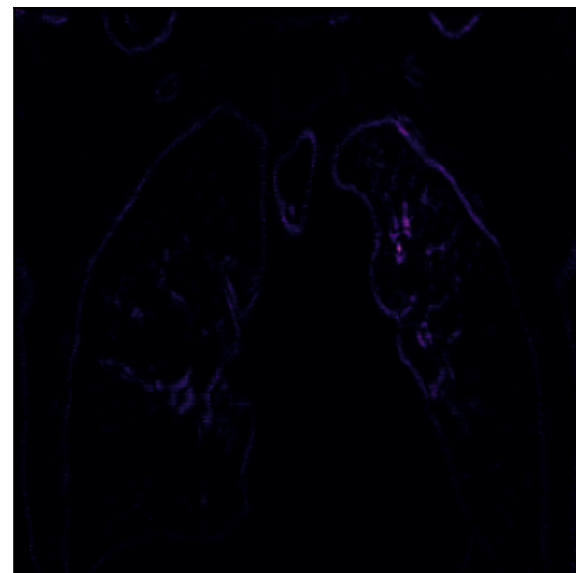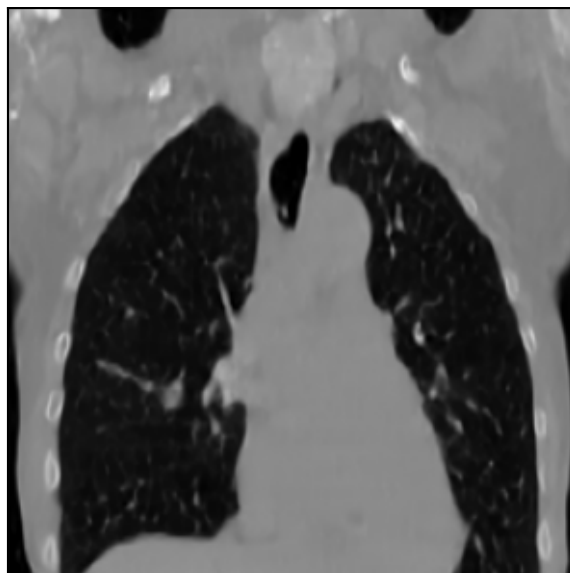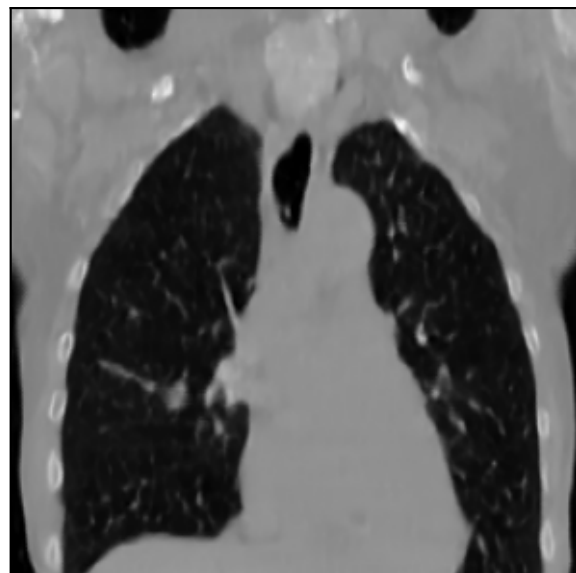

Sagittal mid

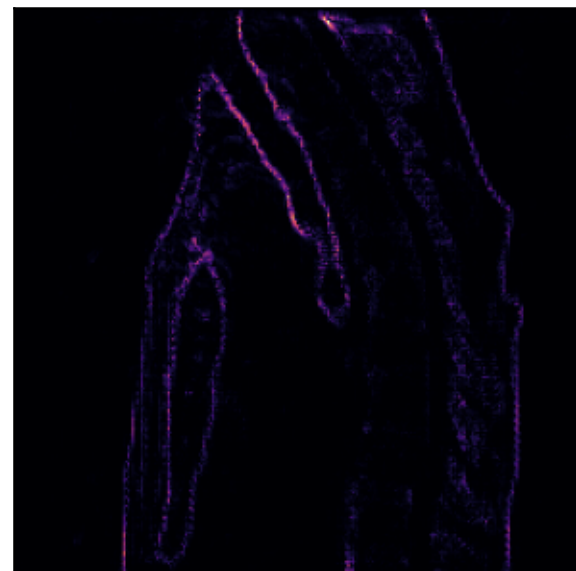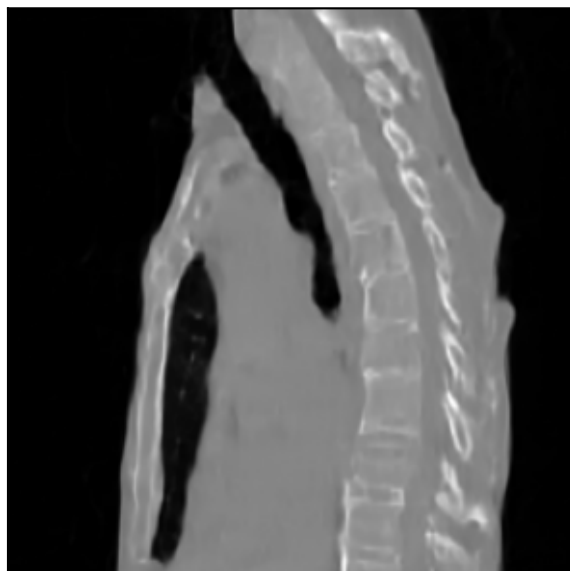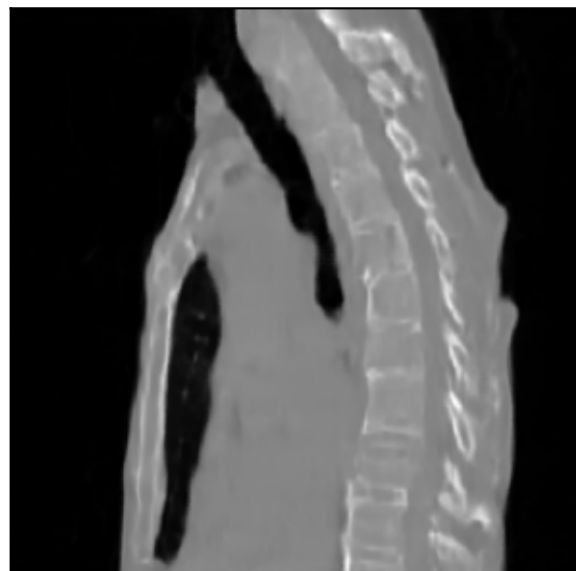

TemporalMotion — details (FAIL)

Metric	Value
jacobian_analysis	list[9]
trajectory_smoothness	0.52824

RobustnessCheck — details (FAIL)

Metric	Value
snr	1.9195796
snr_status	FAIL
fov_status	PASS


GeomIntegrity — details (FAIL)

Metric	Value
drr_ssim	4.9641e-06
drr_ncc	0.28637
z_continuity_score	1
z_issues	list[0]
landmark_deviations_lung_centroid_diff_mm	0.0074933
landmark_deviations_bone_centroid_diff_mm	0.99822

GeomIntegrity — plot_overlay_path

GeomIntegrity: plot_overlay_path

Overlay: Red=Input, Green=DRR

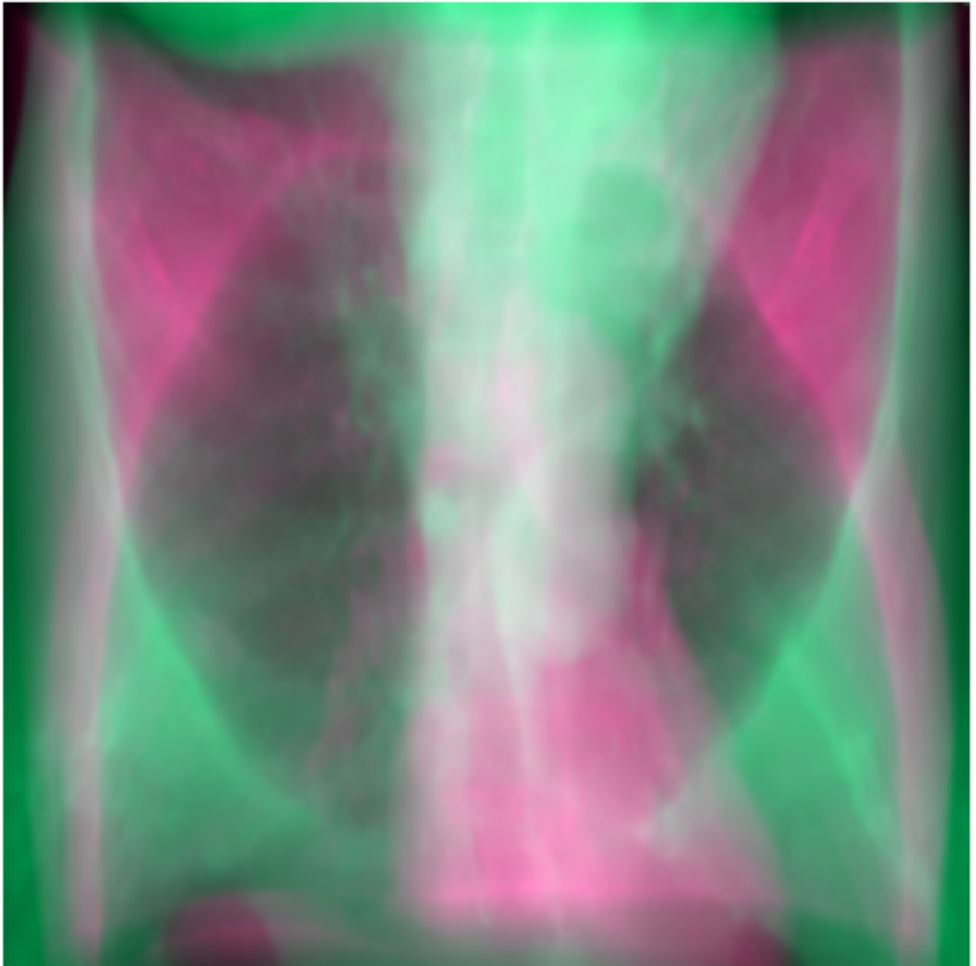

DosimetricAccuracy — details (ERROR)

Metric	Value
status	ERROR
message	Dose distributions missing