


## Module status

### **phase 60 — Module status**


| Module             | Status |
|--------------------|--------|
| TemporalMotion     | FAIL   |
| RobustnessCheck    | FAIL   |
| GeomIntegrity      | FAIL   |
| DosimetricAccuracy | ERROR  |

# CT comparison


Synthetic (warped 50→PP)

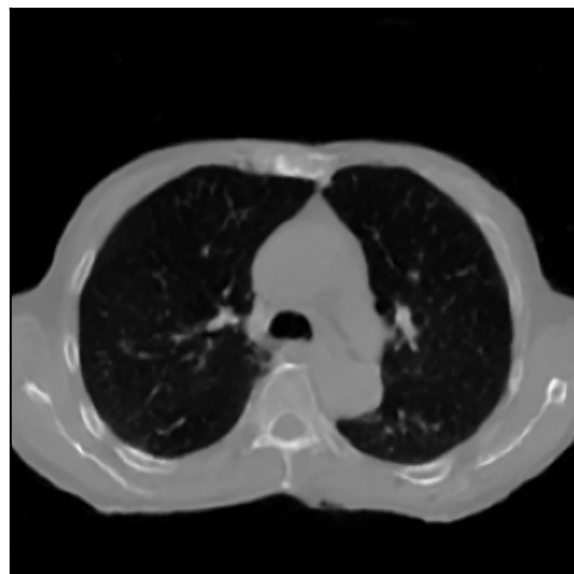

Planning (phase 50)



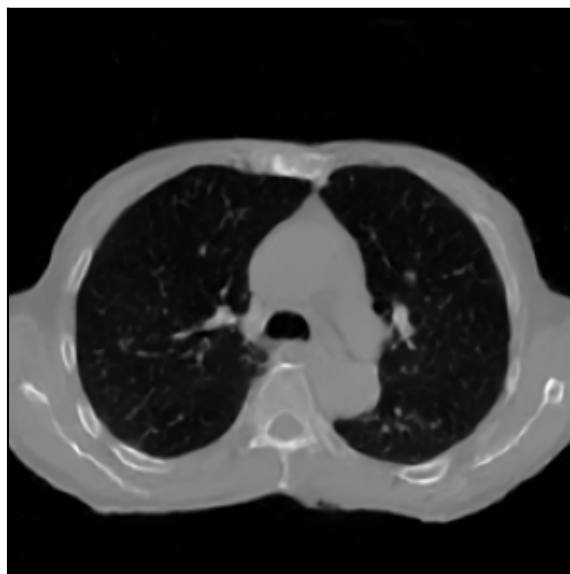


|Synthetic – Planning|



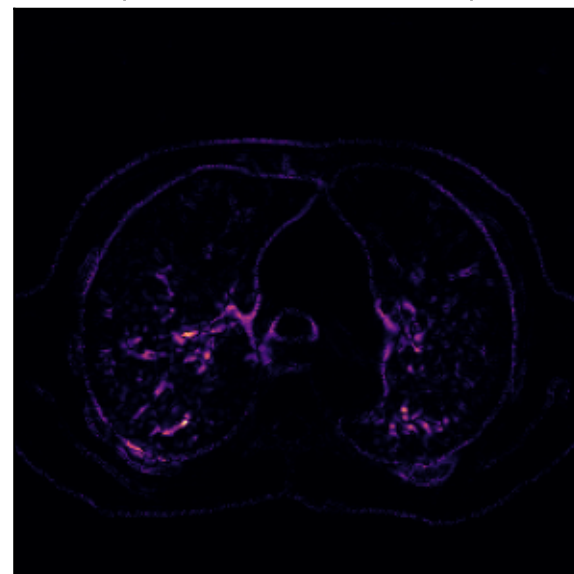


Axial mid

Coronal mid

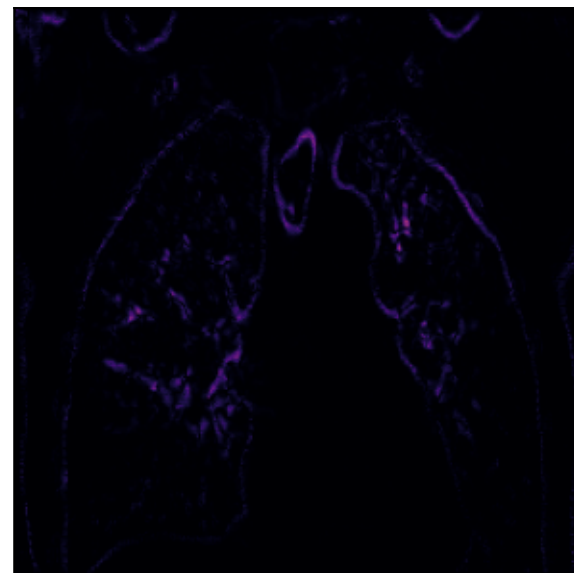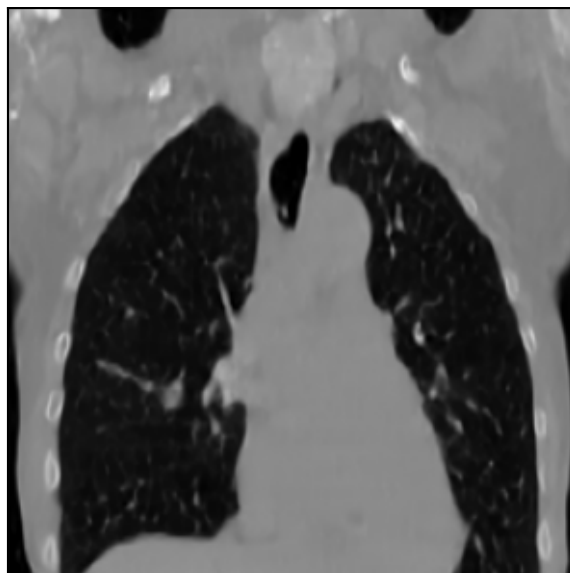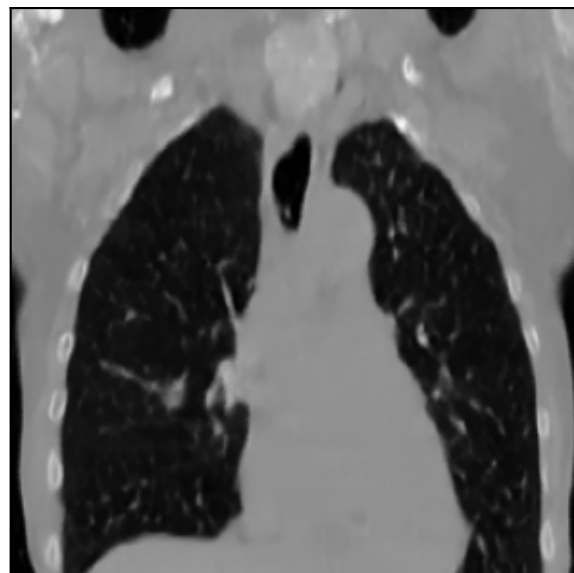

Sagittal mid

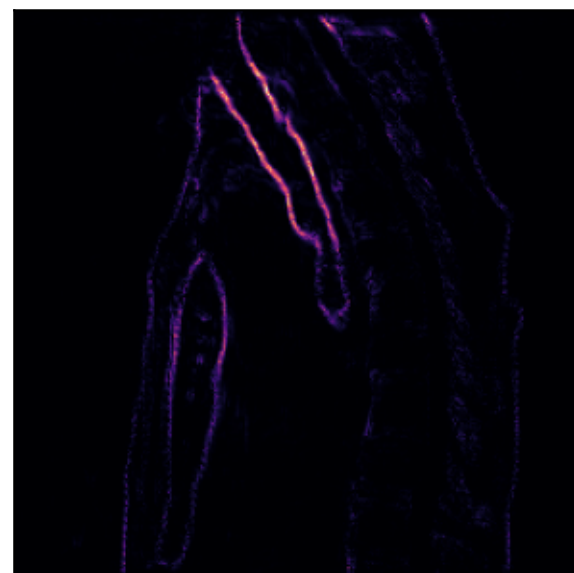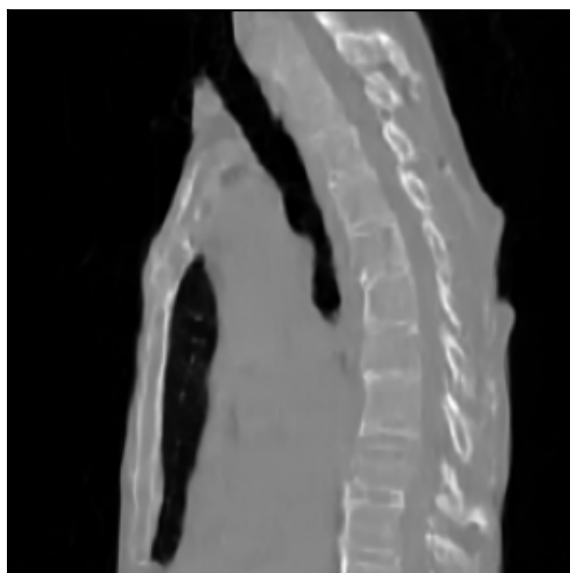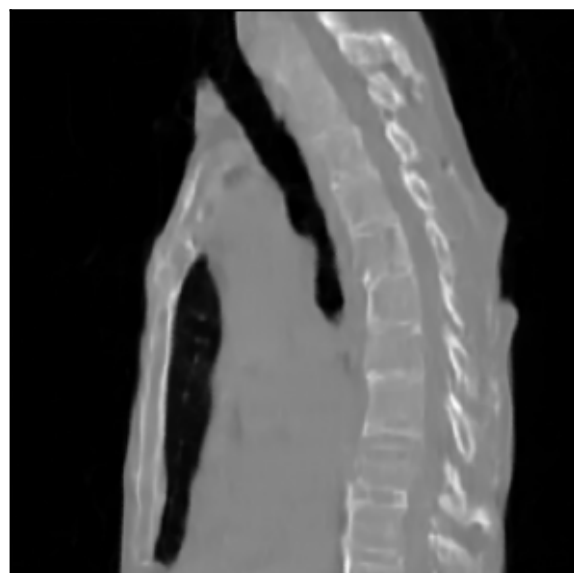

TemporalMotion — details (FAIL)

| Metric                | Value   |
|-----------------------|---------|
| jacobian_analysis     | list[9] |
| trajectory_smoothness | 0.52824 |

RobustnessCheck — details (FAIL)

| Metric     | Value     |
|------------|-----------|
| snr        | 1.9195796 |
| snr_status | FAIL      |
| fov_status | PASS      |


GeomIntegrity — details (FAIL)

| Metric                                    | Value      |
|-------------------------------------------|------------|
| drr_ssim                                  | 5.0108e-06 |
| drr_ncc                                   | 0.28502    |
| z_continuity_score                        | 1          |
| z_issues                                  | list[0]    |
| landmark_deviations_lung_centroid_diff_mm | 0.02913    |
| landmark_deviations_bone_centroid_diff_mm | 0.94248    |

GeomIntegrity — plot\_overlay\_path

GeomIntegrity: plot\_overlay\_path

Overlay: Red=Input, Green=DRR

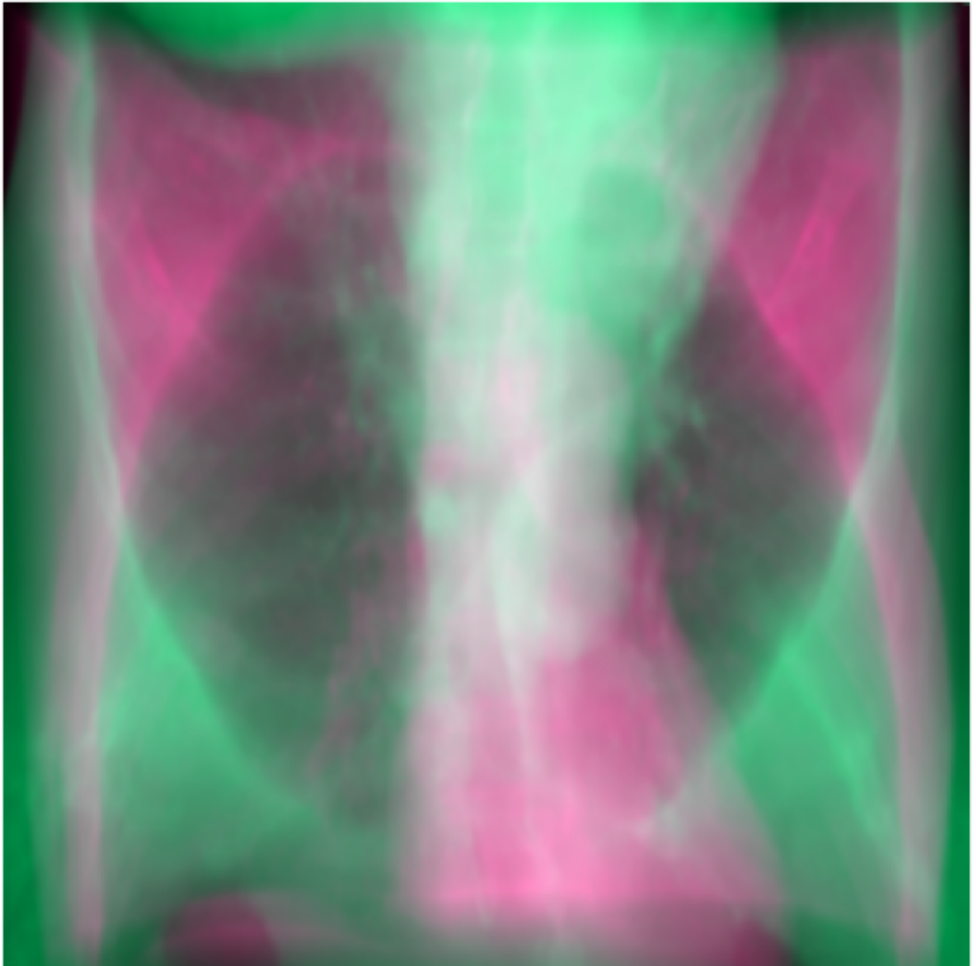

DosimetricAccuracy — details (ERROR)

| Metric  | Value                      |
|---------|----------------------------|
| status  | ERROR                      |
| message | Dose distributions missing |