


Newton-Gauss vs L-BFGS: Speed and Accuracy

Calibration Speed



v_0 Recovery Error

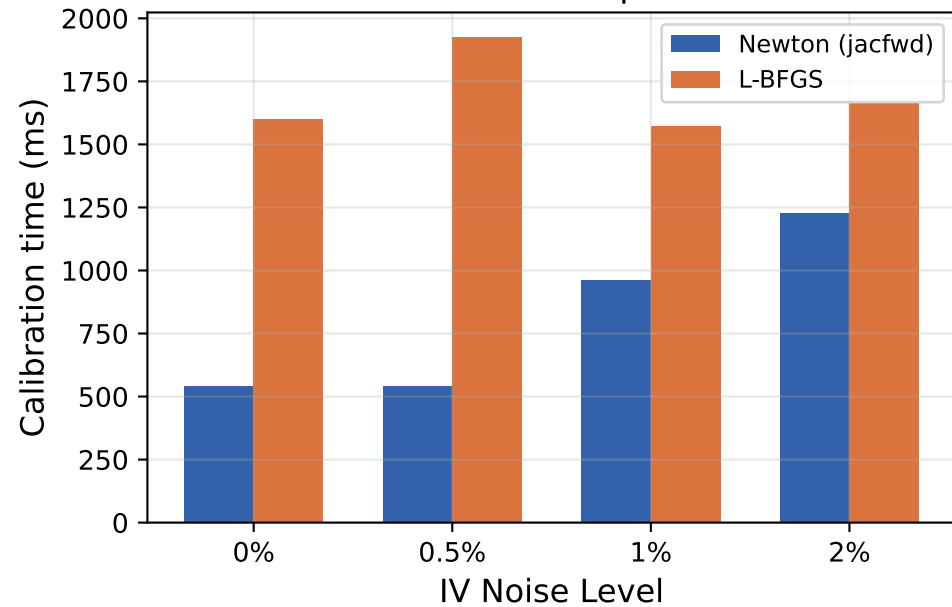