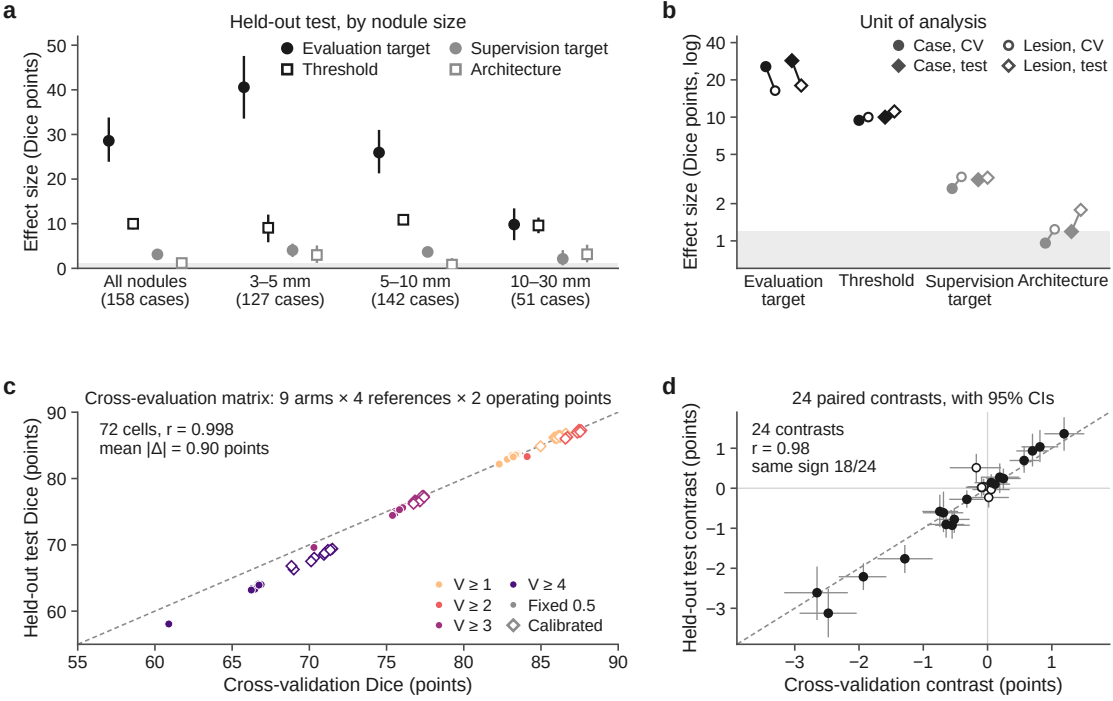
a
Held-out test, by nodule size
Evaluation target
Threshold
Supervision target
Architecture
Effect size (Dice points)
50
40
30
20
10
0
All nodules
(158 cases)
3–5 mm
(127 cases)
5–10 mm
(142 cases)
10–30 mm
(51 cases)
b
Unit of analysis
Case, CV
Case, test
Lesion, CV
Lesion, test
Effect size (Dice points, log)
40
20
10
5
2
1
Evaluation target
Threshold
Supervision target
Architecture
c
Cross-evaluation matrix: 9 arms × 4 references × 2 operating points
72 cells, r = 0.998
mean |Δ| = 0.90 points
Held-out test Dice (points)
90
80
70
60
55
60
65
70
75
80
85
90
Cross-validation Dice (points)
V ≥ 1
V ≥ 2
V ≥ 3
V ≥ 4
Fixed 0.5
Calibrated
d
24 paired contrasts, with 95% CIs
24 contrasts
r = 0.98
same sign 18/24
Held-out test contrast (points)
1
0
−1
−2
−3
Cross-validation contrast (points)