

Controlled scientific extraction sample

Synthetic data for parser verification; not an empirical research result.

1. Evaluation protocol

We evaluate on the held-out Test split with 200 examples per method.
Accuracy is reported in percent. Uncertainty denotes standard deviation.

Table 1. Accuracy on the Test split over three independent runs.

Method	Split	Accuracy (%)	SD
Baseline A	Test	80.0	1.2
Method B	Test	85.5	0.8

Note: SD is measured across runs, not a confidence interval.

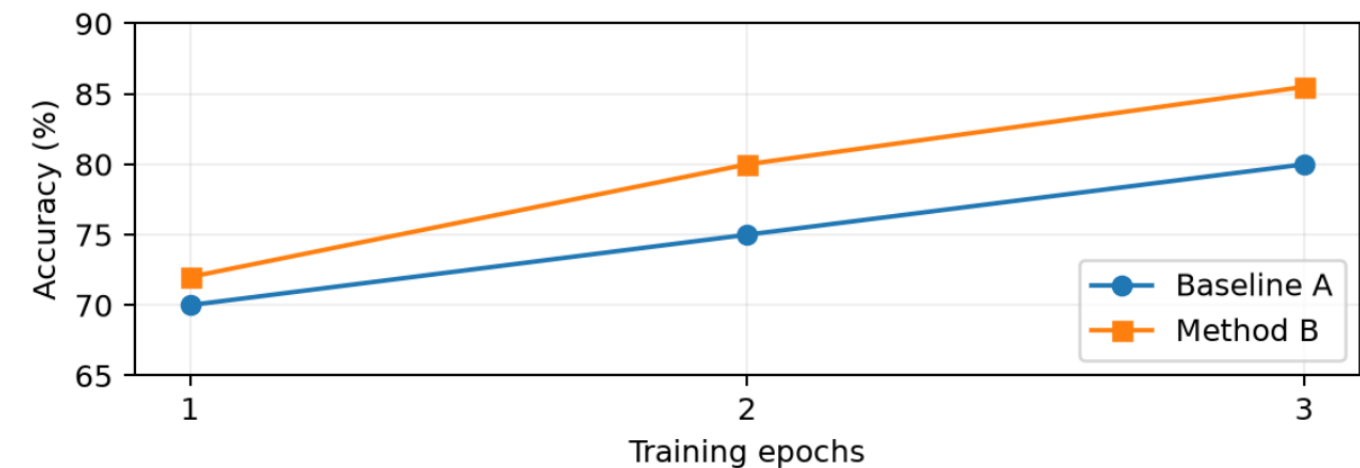


Figure 1. Test accuracy at three training epochs. Points are means.

2. Accuracy definition

$$A = \frac{100}{N} \sum_{i=1}^N \mathbf{1}(\hat{y}_i = y_i)$$

Here N is the number of test examples; y is the reference label.
The indicator is 1 for a correct predicted label and 0 otherwise.