




Filename: 2024-11-21 - 15.05.46.D5000

Sample Info

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	78.7	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder
B1	8.01	MdecD1		Caution! Expired ScreenTape device (used after two weeks of first use)
C1	0.276	McavF1		Caution! Expired ScreenTape device (used after two weeks of first use); Peak out of Sizing Range


Compact Peak Table

Well	Sample Description	Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
A1	Ladder	15	8.81	-	904	-		Lower Marker
A1	Ladder	100	9.01	-	139	11.45		
A1	Ladder	250	10.0	-	61.6	12.72		
A1	Ladder	400	10.2	-	39.1	12.93		
A1	Ladder	600	10.8	-	27.7	13.72		
A1	Ladder	1000	10.9	-	16.8	13.88		
A1	Ladder	1500	10.3	-	10.5	13.07		
A1	Ladder	2500	7.95	-	4.89	10.11		
A1	Ladder	3500	5.93	-	2.60	7.53		
A1	Ladder	5000	3.60	-	1.11	4.58		
A1	Ladder	10000	3.25	3.25	0.500	-		Upper Marker
B1	MdecD1	15	7.13	-	731	-		Lower Marker
B1	MdecD1	285	8.01	-	43.2	100.00		
B1	MdecD1	10000	3.25	3.25	0.500	-		Upper Marker
C1	McavF1	15	6.57	-	674	-		Lower Marker
C1	McavF1	158	0.203	-	1.98	73.75		
C1	McavF1	10000	3.25	3.25	0.500	-		Upper Marker
C1	McavF1	63650	0.0723	-	0.00175	26.25		Peak outside of Sizing Range



Default image (Contrast 100%)

A1: Ladder

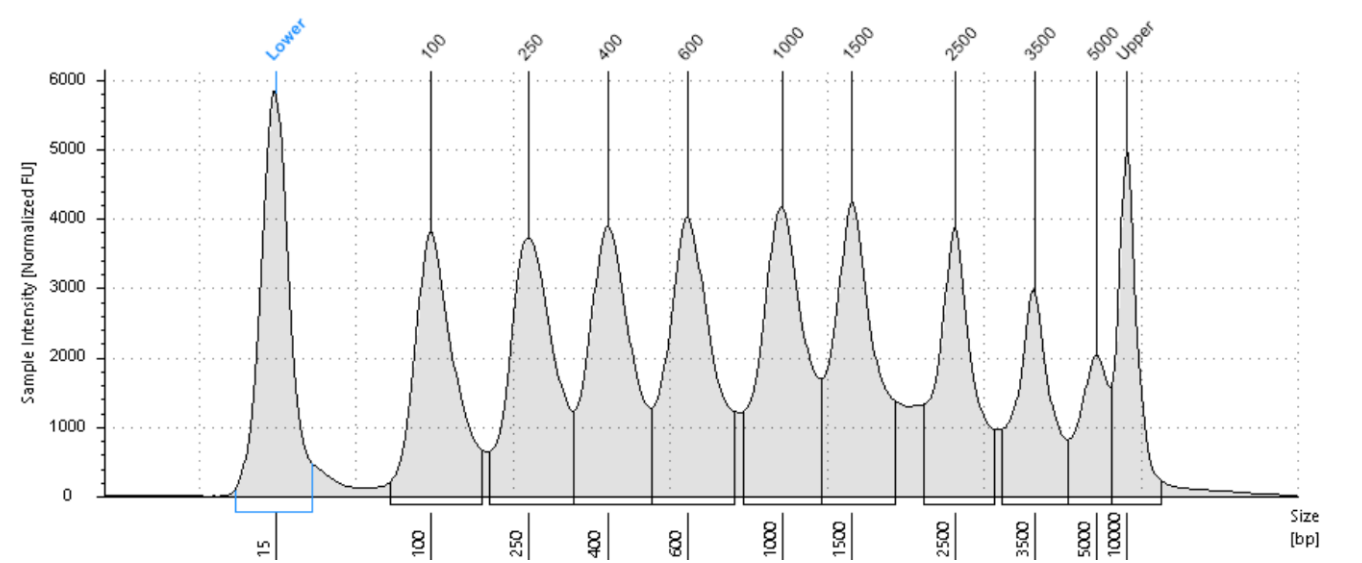


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	78.7	Ladder		Caution! Expired ScreenTape device (used after two weeks of first use); Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	8.81	-	904	-		Lower Marker
100	9.01	-	139	11.45		
250	10.0	-	61.6	12.72		
400	10.2	-	39.1	12.93		
600	10.8	-	27.7	13.72		
1000	10.9	-	16.8	13.88		
1500	10.3	-	10.5	13.07		
2500	7.95	-	4.89	10.11		
3500	5.93	-	2.60	7.53		
5000	3.60	-	1.11	4.58		
10000	3.25	3.25	0.500	-		Upper Marker

B1: MdecD1

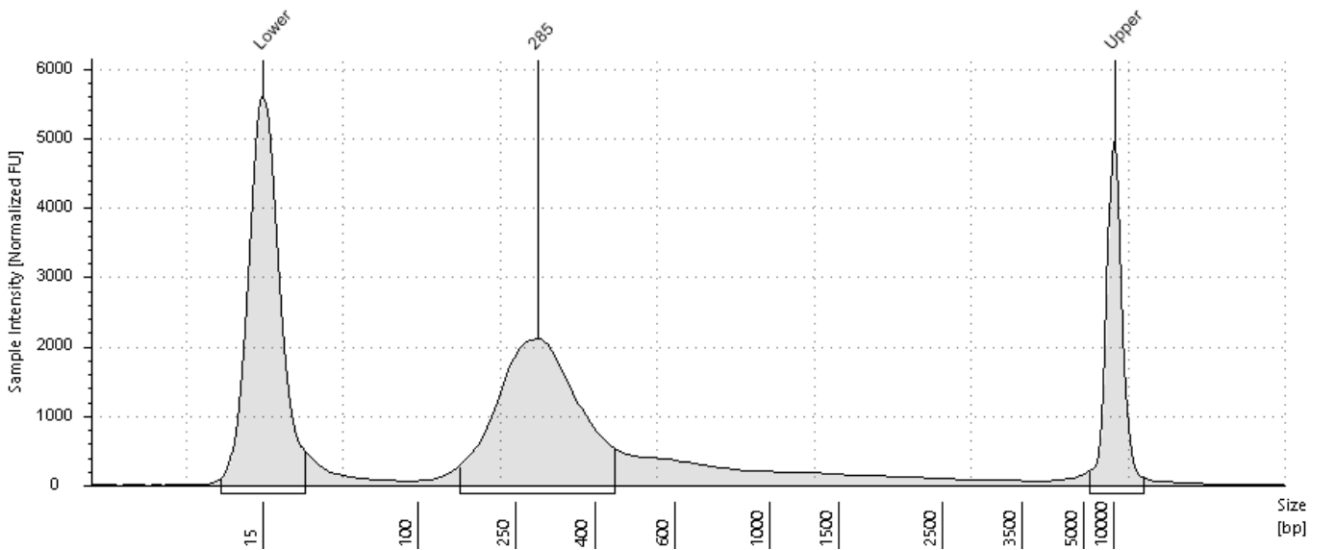


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	8.01	MdecD1		Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.13	-	731	-		Lower Marker
285	8.01	-	43.2	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C1: McavF1

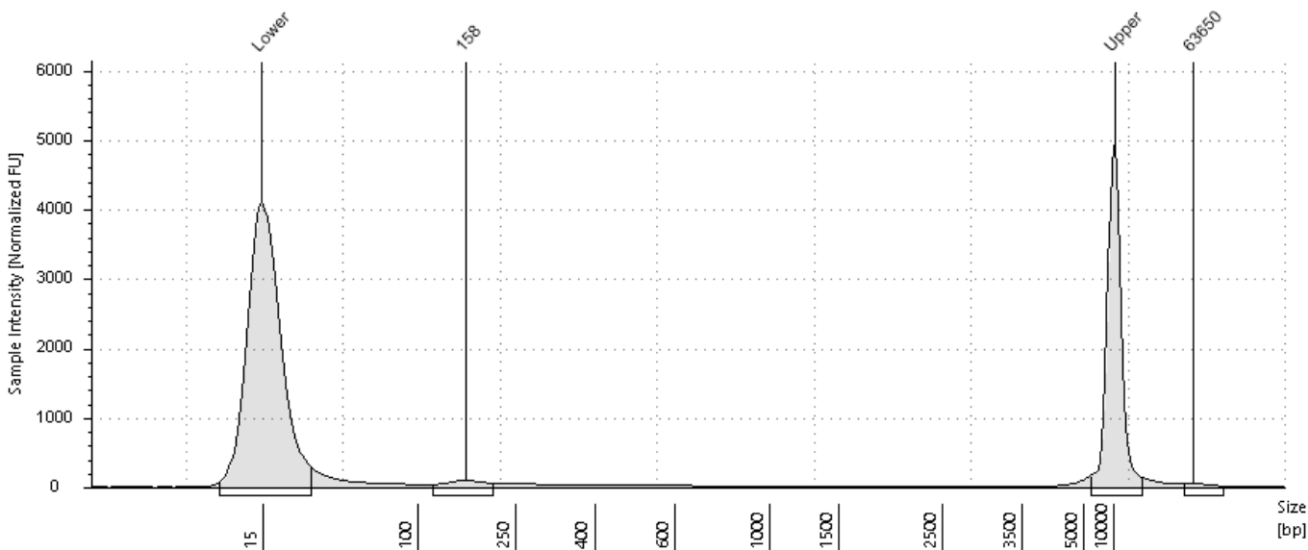

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C1	0.276	McavF1		Caution! Expired ScreenTape device (used after two weeks of first use); Peak out of Sizing Range

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.57	-	674	-		Lower Marker
158	0.203	-	1.98	73.75		
10000	3.25	3.25	0.500	-		Upper Marker
63650	0.0723	-	0.00175	26.25		Peak outside of Sizing Range