




Filename: 2024-11-19 - 10.10.32.RNA

Sample Info

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	-	-	75.7	Ladder		Caution! Expired ScreenTape device; Ladder
B1	9.0	0.9	28.3	Pcomp_E10_2		Caution! Expired ScreenTape device


Compact Peak Table

Well	Sample Description	Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
A1	Ladder	25	40.0	40.0	4710	-		Lower Marker
A1	Ladder	200	7.52	-	111	11.56		
A1	Ladder	500	15.0	-	87.9	23.00		
A1	Ladder	1000	10.6	-	31.3	16.37		
A1	Ladder	2000	11.3	-	16.6	17.41		
A1	Ladder	4000	10.9	-	7.99	16.72		
A1	Ladder	6000	9.72	-	4.76	14.95		
B1	Pcomp E10 2	25	40.0	40.0	4710	-		Lower Marker
B1	Pcomp E10 2	1865	7.30	-	11.5	51.40		18S
B1	Pcomp E10 2	3942	6.91	-	5.15	48.60		28S

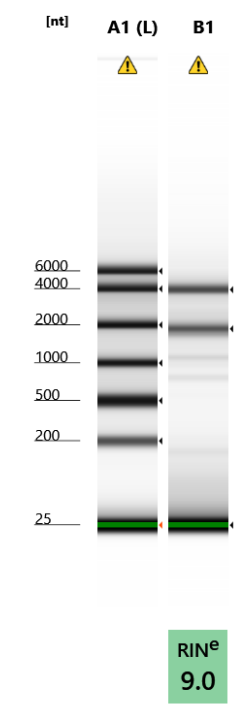

Default image (Contrast 100%)

A1: Ladder

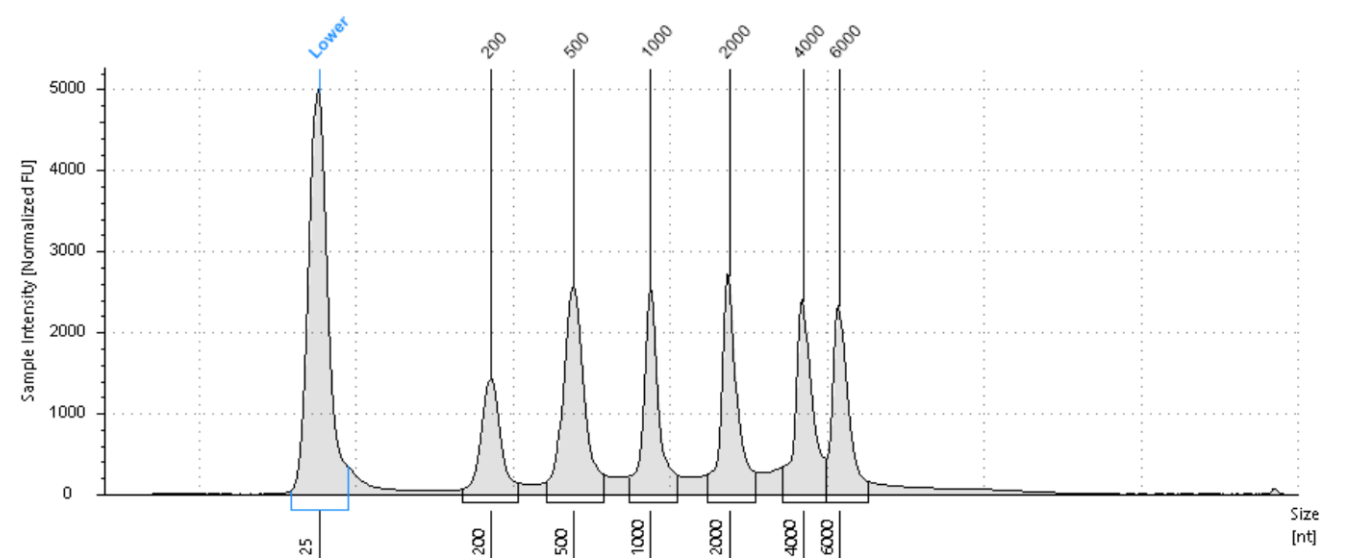


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	-	-	75.7	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
200	7.52	-	111	11.56		
500	15.0	-	87.9	23.00		
1000	10.6	-	31.3	16.37		
2000	11.3	-	16.6	17.41		
4000	10.9	-	7.99	16.72		
6000	9.72	-	4.76	14.95		

B1: Pcomp_E10_2

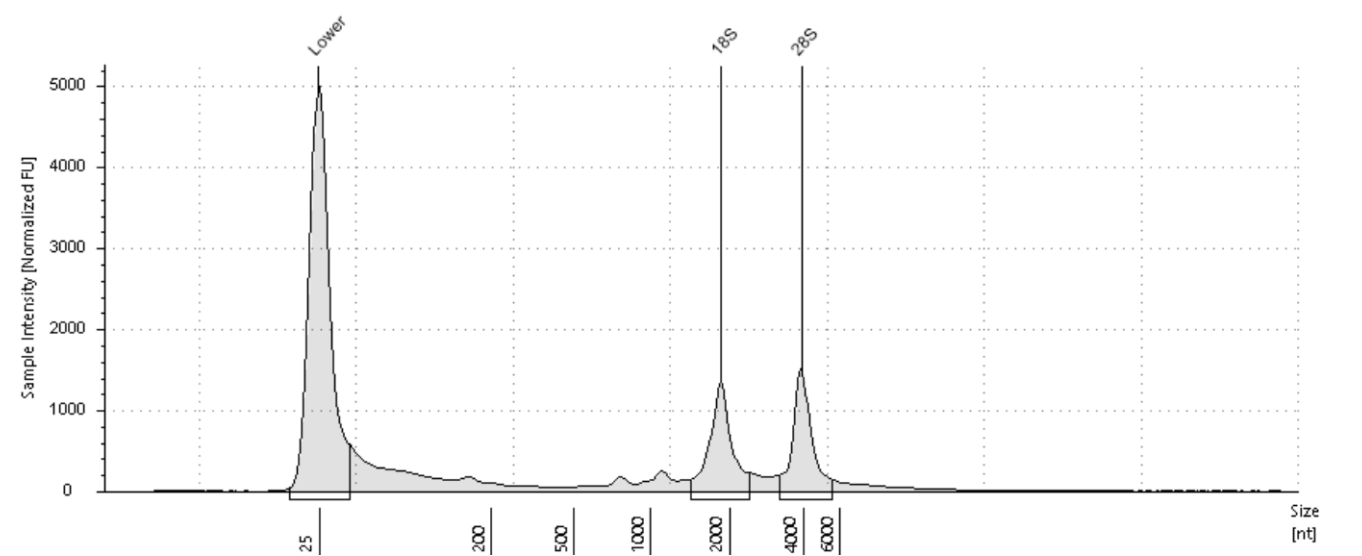

Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	9.0	0.9	28.3	Pcomp_E10_2		Caution! Expired ScreenTape device

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1865	7.30	-	11.5	51.40		18S
3942	6.91	-	5.15	48.60		28S