EUROPEAN PATENT OFFICE

Patent Abstracts of Japan

PUBLICATION NUMBER : 08136660
PUBLICATION DATE : 31-05-96

APPLICATION DATE : 08-11-94
APPLICATION NUMBER : 06273276

APPLICANT : ALOKA CO LTD;

INVENTOR : IIDA TAKAO;

INT.CL. : G01T 1/185 G01T 1/167 G01T 7/02 H01J 47/02

TITLE : RADIOACTIVE RAY MEASURING INSTRUMENT

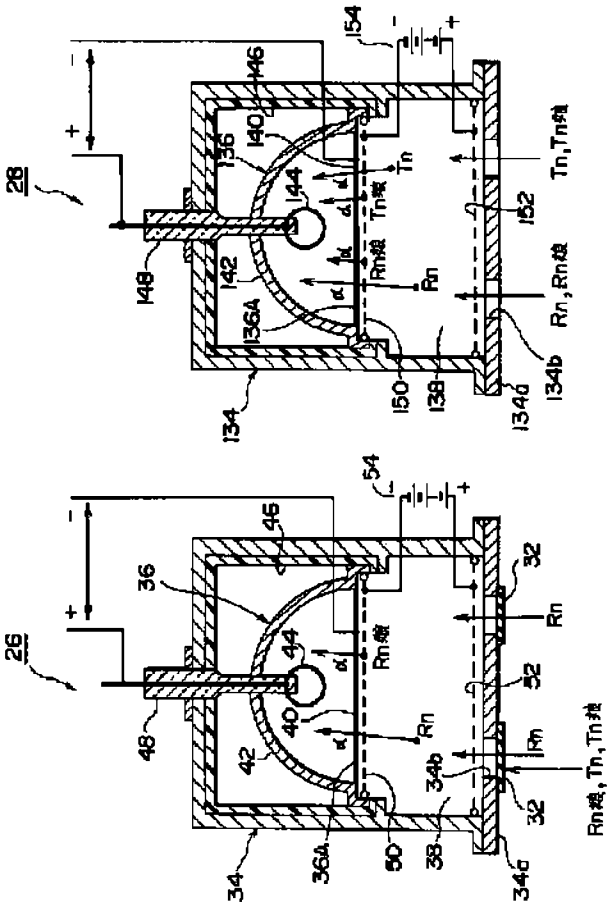

ABSTRACT : PURPOSE: To individually measure radon and thoron, measure radon daughter nuclide and thoroin daughter nuclide in real time, and further improve the measurement sensitivity of the magnetized nuclide.

CONSTITUTION: In a first detection unit 26, only radon is introduced into a gas introduction chamber 38 by a radon extraction filter 32. Since the radon daughter nuclide generated due to the decay in the gas introduction chamber 38 is a magnetized nuclide, it is captured by an electrode at one side. α ray from the radon and radon daughter nuclide is detected by an ionization box 36 via an α ray incidence window 36A. On the other hand, all of the radon and its daughter nuclide and thoron and its daughter nuclide are introduced into a second detection unit 28 and the radon daughter nuclide and thoron daughter nuclide are captured by an electrode 150 at one side. In an ionization box 136, α rays from the radon and its daughter nuclide and thoron and its daughter nuclide are detected.

COPYRIGHT: (C)1996,JPO