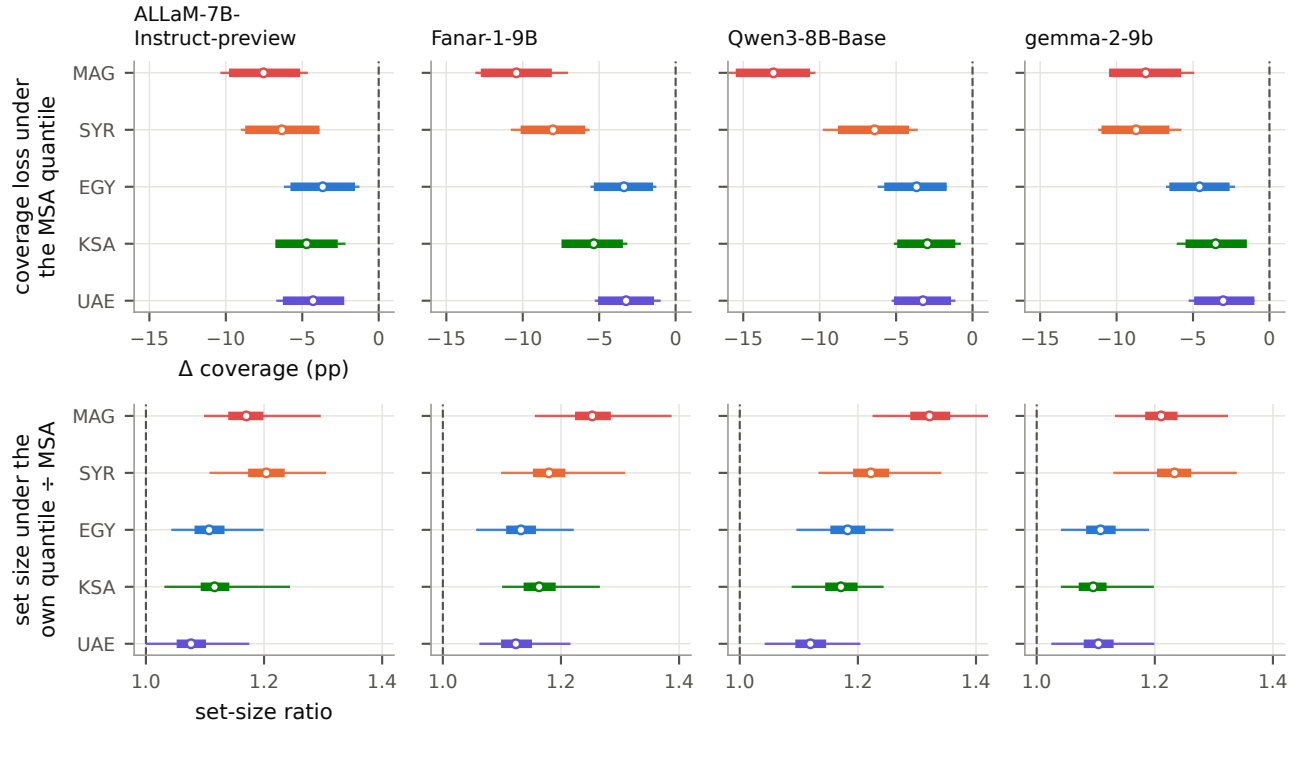
ALLaM-7B-Instruct-preview
Fanar-1-9B
Qwen3-8B-Base
gemma-2-9b
coverage loss under the MSA quantile
MAG
SYR
EGY
KSA
UAE
−15
−10
−5
0
Δ coverage (pp)
set size under the own quantile ÷ MSA
1.0
1.2
1.4
set-size ratio
95% interval, calibration sample fixed (B = 2000)
95% interval, calibration and test resampled with q̂ re-selected (B = 1000)