


Controlled F0/F1 reranking ablation

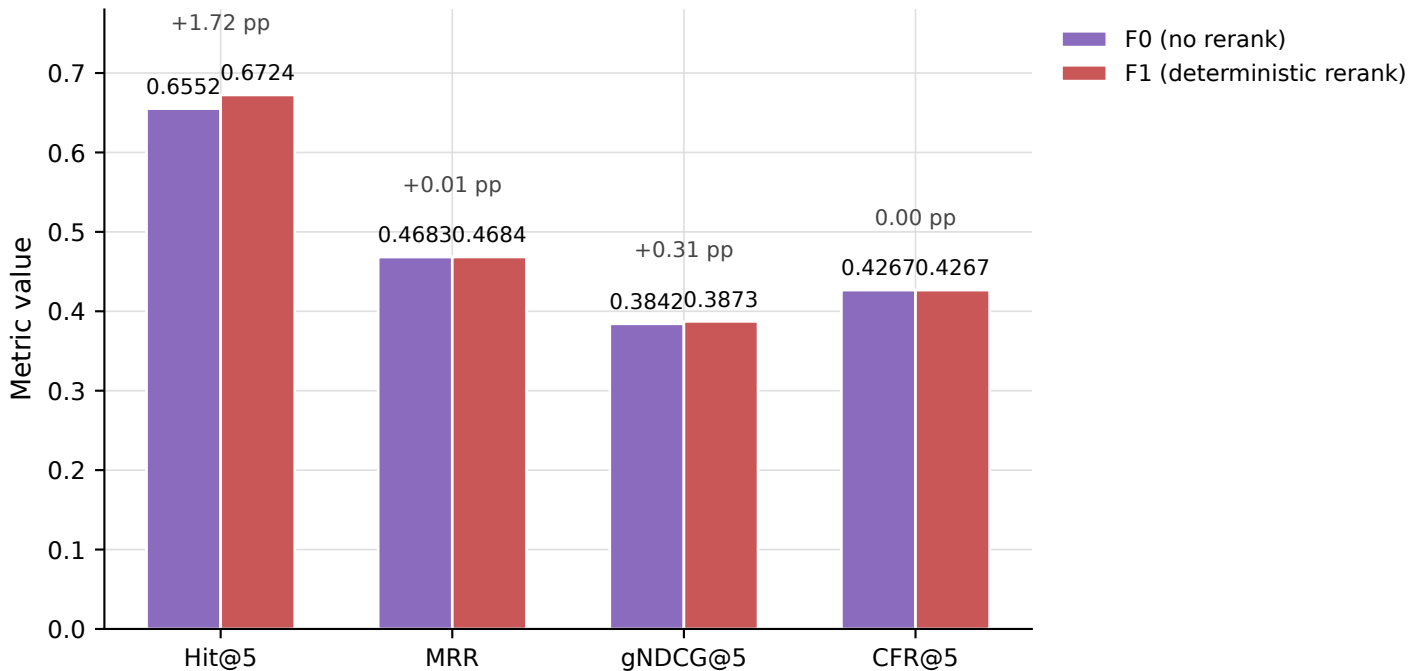

Both systems use the same hybrid RRF top-50 candidate pool; only reranking is toggled.