A 3D candidate must also look like a chromatographic peak

After basin-level gates, inspect the extracted ion chromatogram (EIC) around each candidate.

Localised peak

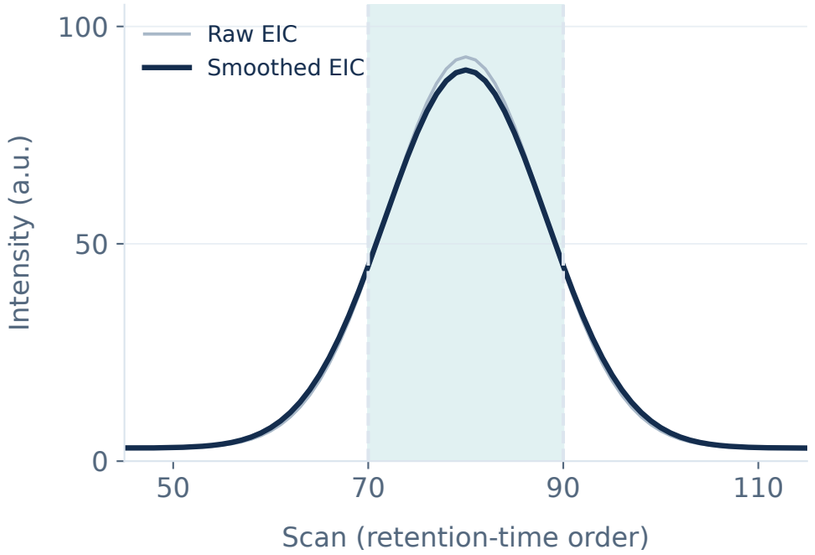

PASS chromatogram check

A maximum lies inside the bounds and rises clearly above the noise.

Fragment of a rising signal

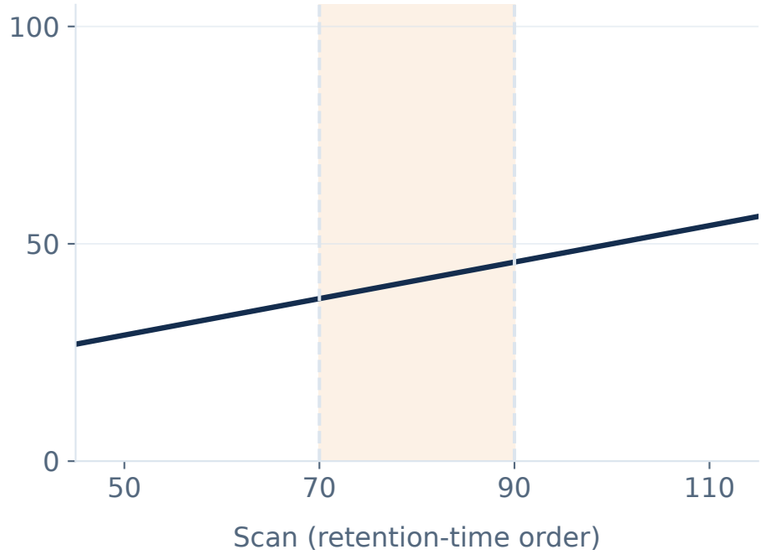

REJECT: no local apex

The signal keeps rising through the candidate's entire interval.

Weak ripple on background

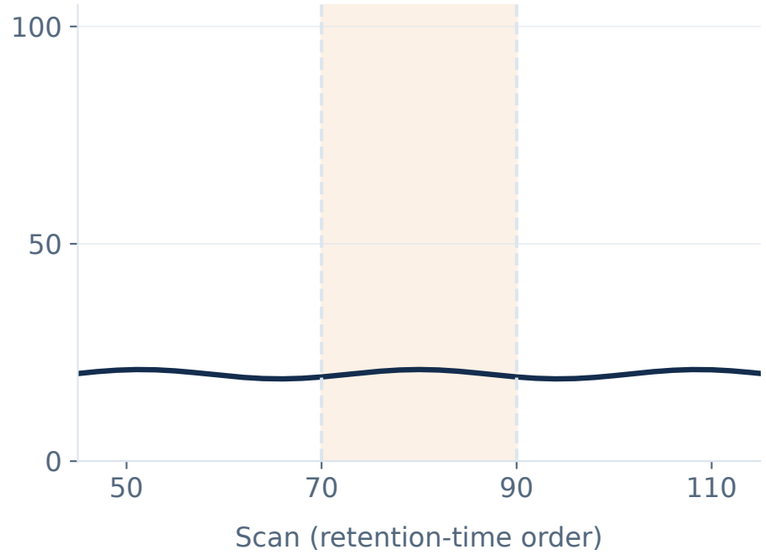

REJECT: too little prominence

A maximum exists, but its prominence is below 3 × the noise reference.

Shaded interval = candidate bounds. Other checks cover scan support, width, m/z consistency, background and score.

3D basins propose candidates; chromatogram checks help reject fragments and noise.

Synthetic candidates passed to the actual EIC check • these are check outcomes, not final feature calls