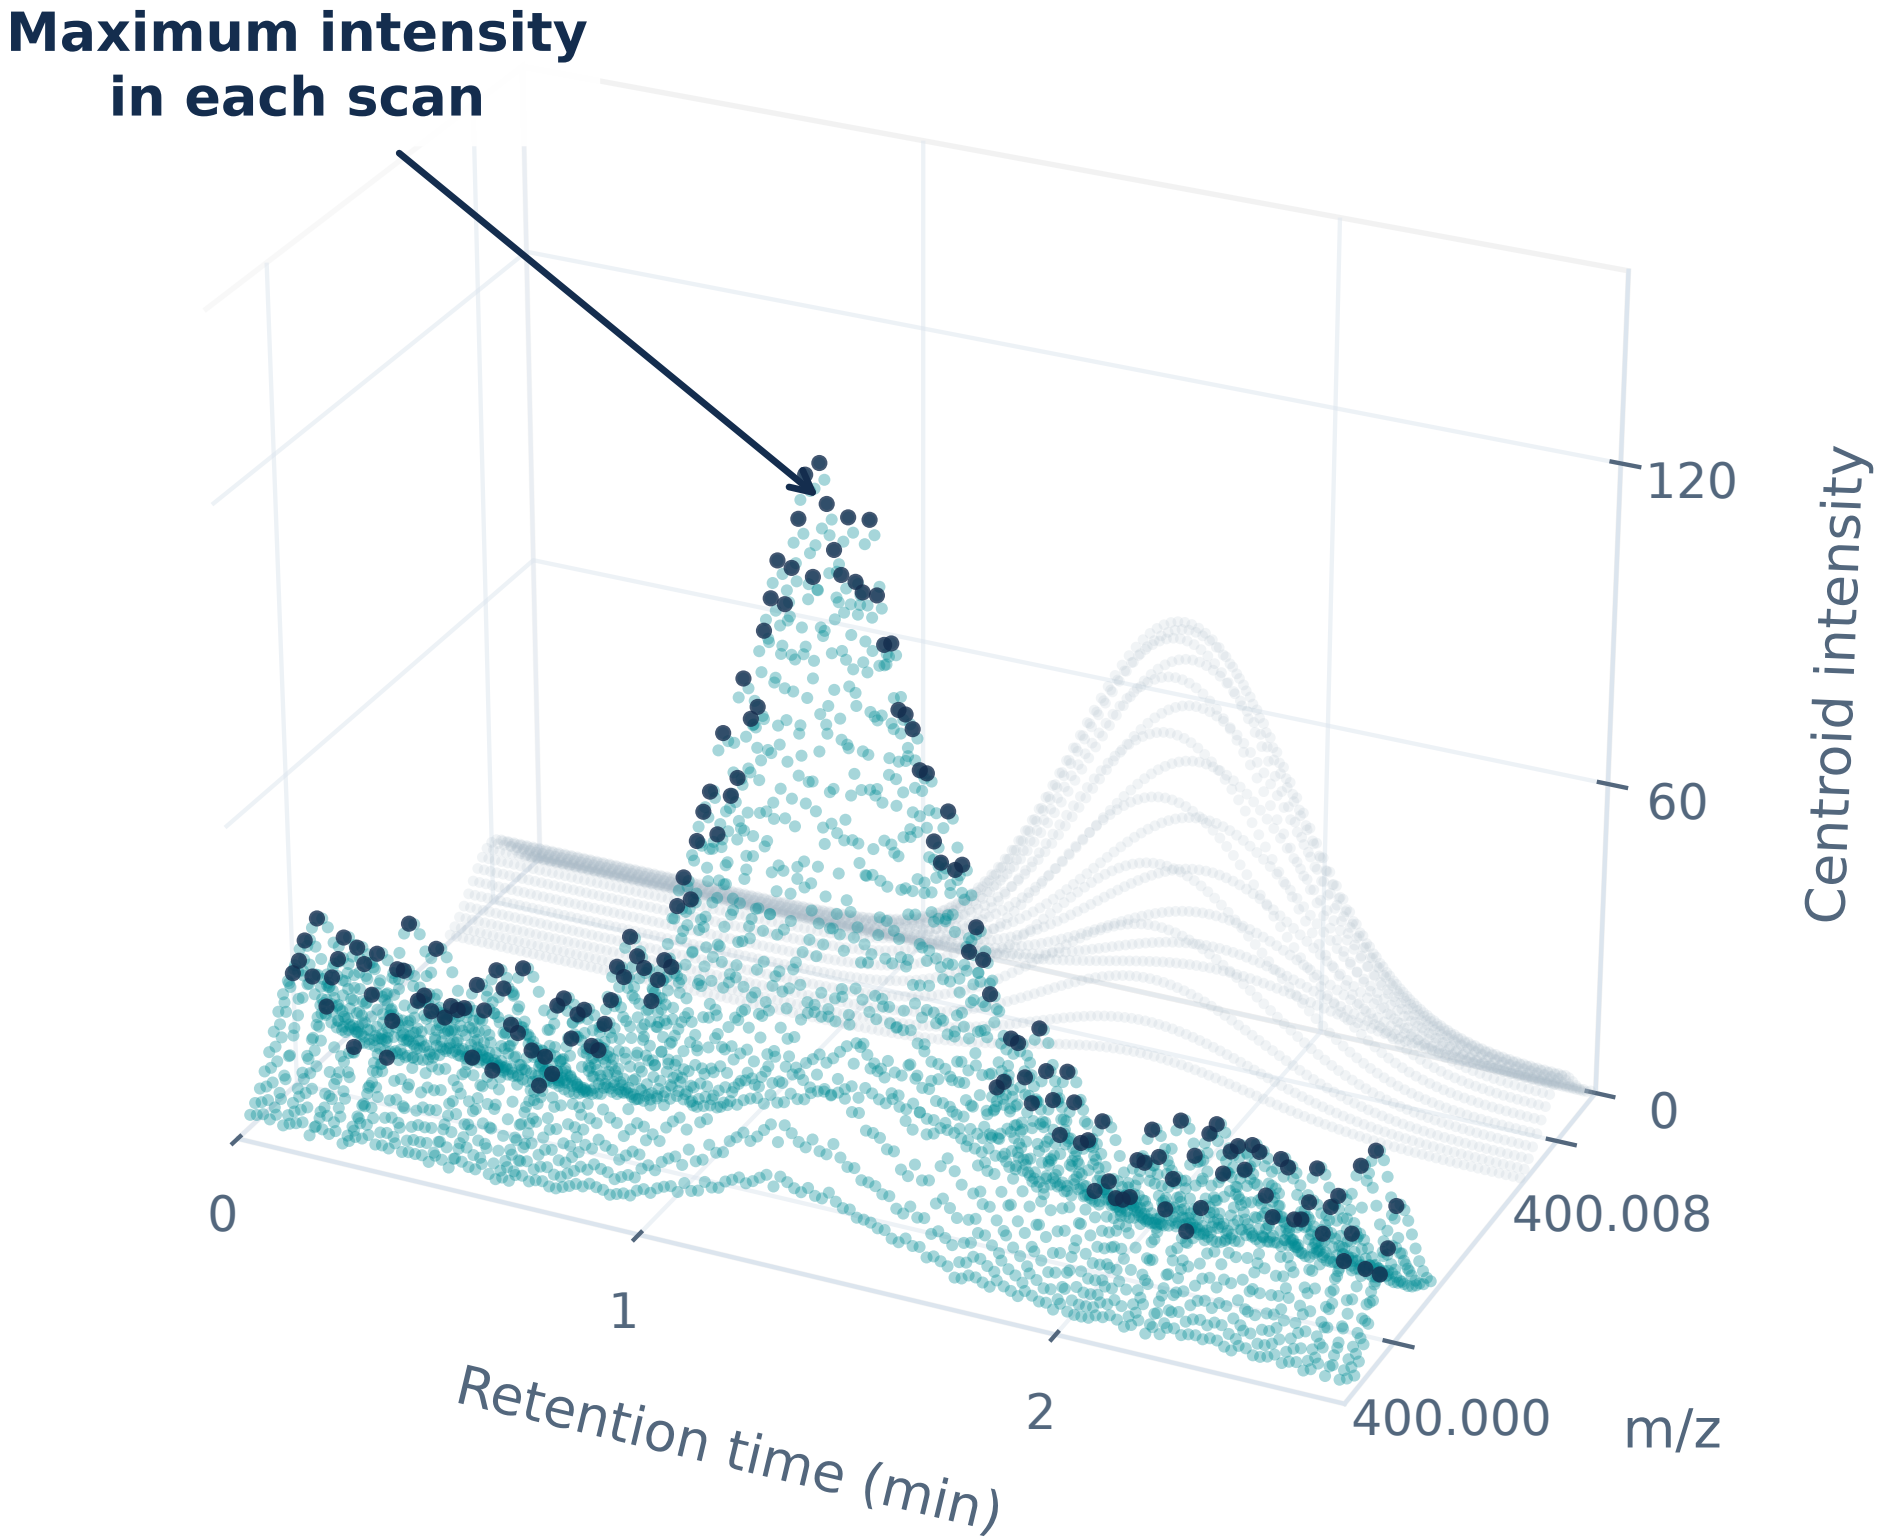

Maximum intensity
in each scan
120
60
0
Centroid intensity
0
1
2
Retention time (min)
400.008
400.000
m/z