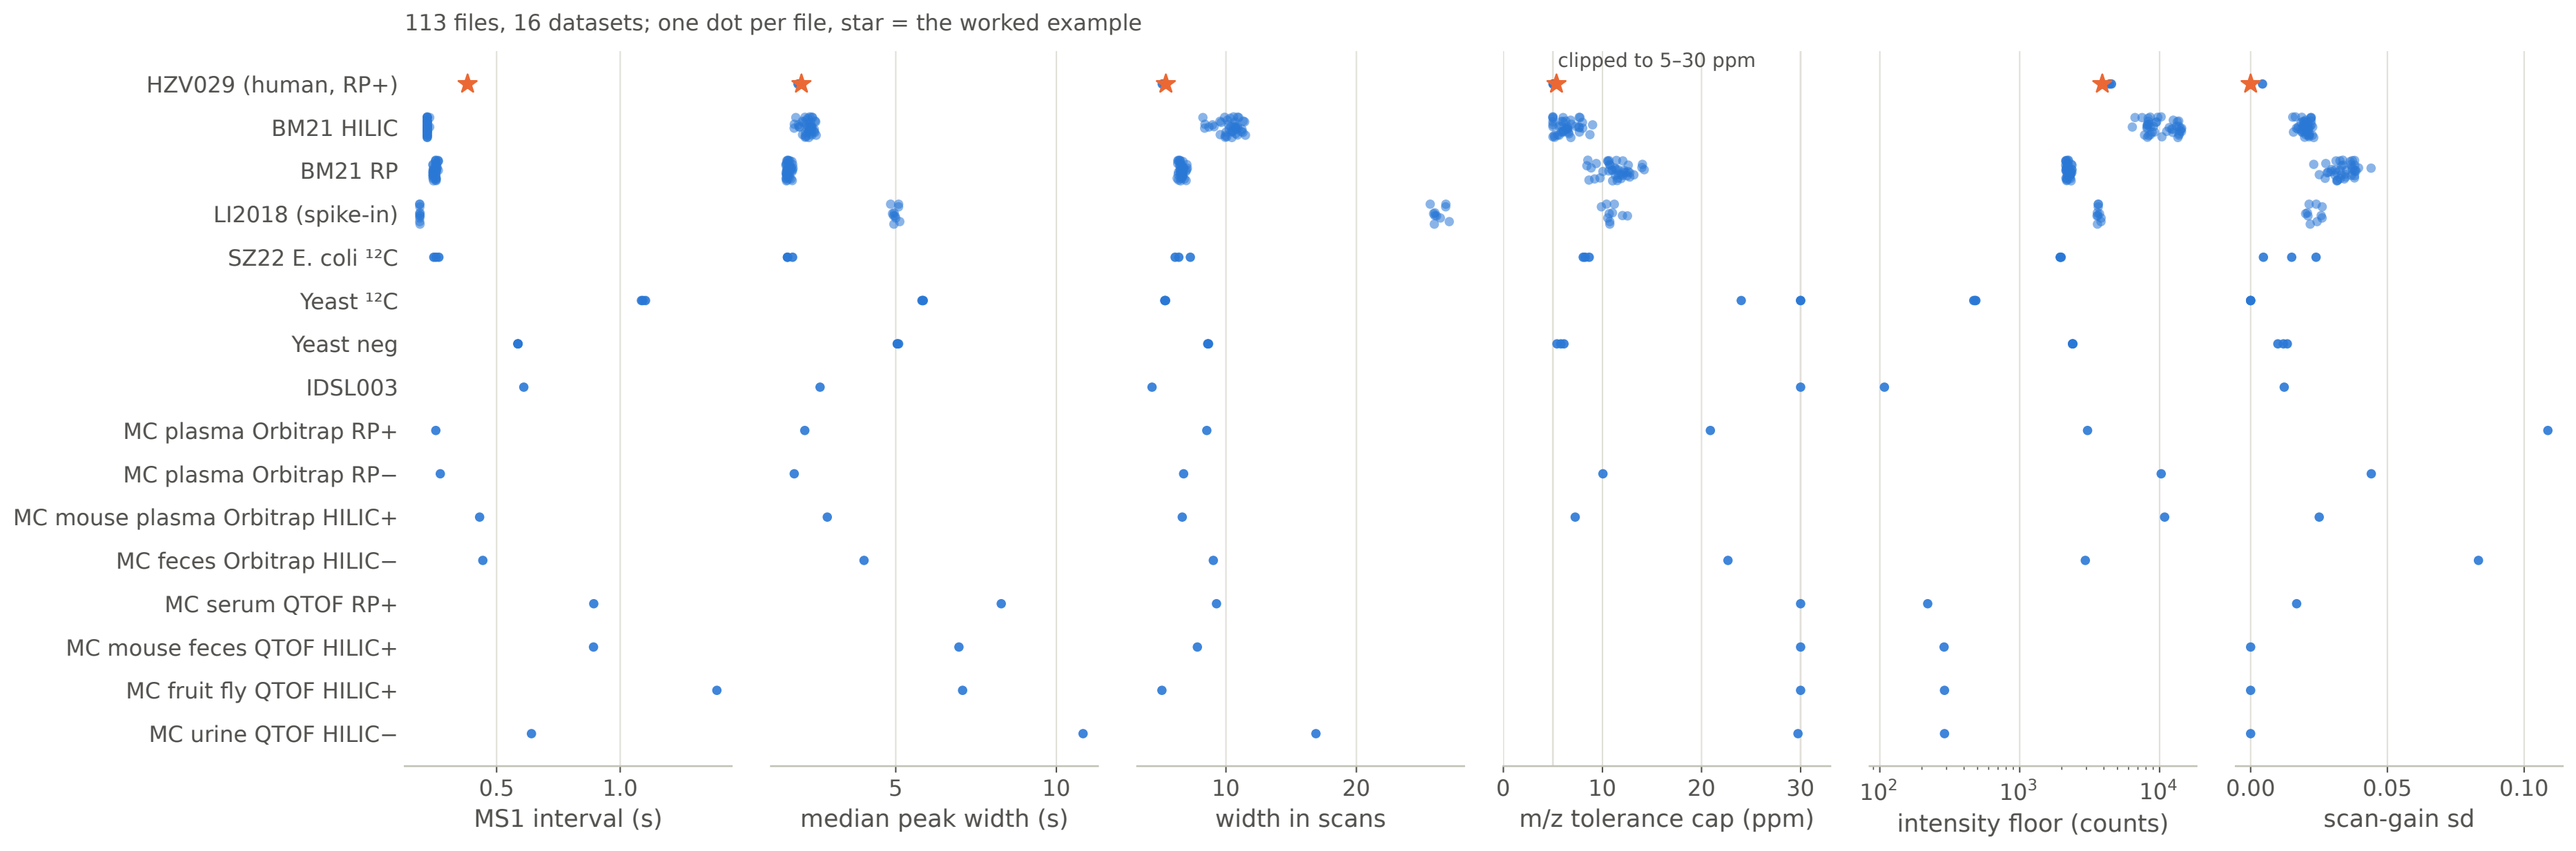
113 files, 16 datasets; one dot per file, star = the worked example
HZV029 (human, RP+)
BM21 HILIC
BM21 RP
LI2018 (spike-in)
SZ22 E. coli ¹²C
Yeast ¹²C
Yeast neg
IDSL003
MC plasma Orbitrap RP+
MC plasma Orbitrap RP−
MC mouse plasma Orbitrap HILIC+
MC feces Orbitrap HILIC−
MC serum QTOF RP+
MC mouse feces QTOF HILIC+
MC fruit fly QTOF HILIC+
MC urine QTOF HILIC−
0.5
1.0
MS1 interval (s)
5
10
median peak width (s)
10
20
width in scans
clipped to 5–30 ppm
0
10
20
30
m/z tolerance cap (ppm)
10^2
10^3
10^4
intensity floor (counts)
0.00
0.05
0.10
scan-gain sd