
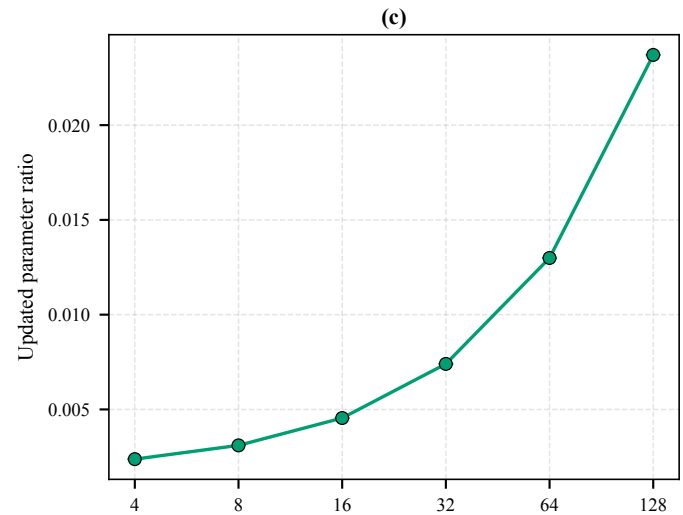
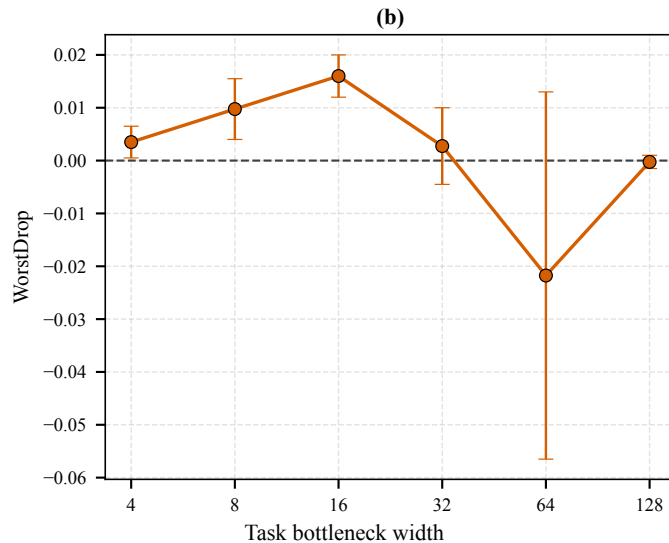


PALL-Adapter task-bottleneck ablation — CIFAR-10

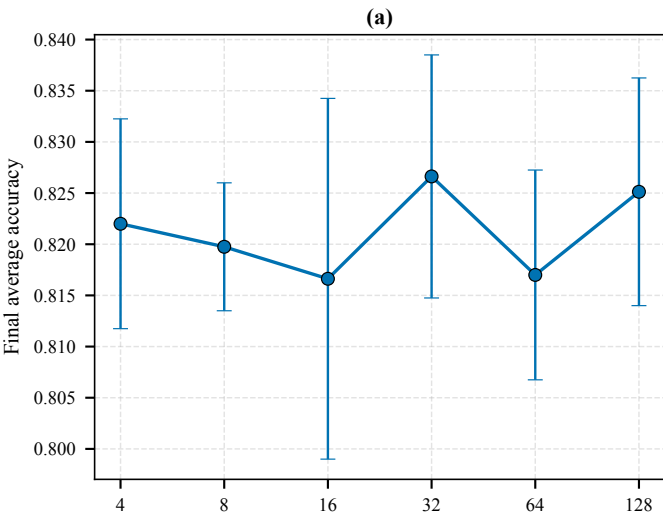

Descriptive, two-seed ablation; non-monotone trends