



OBSonix - in-domain foundation model for fetal ultrasound


(a) In-domain SSL pretraining (LeJEPA, final=0.0811)

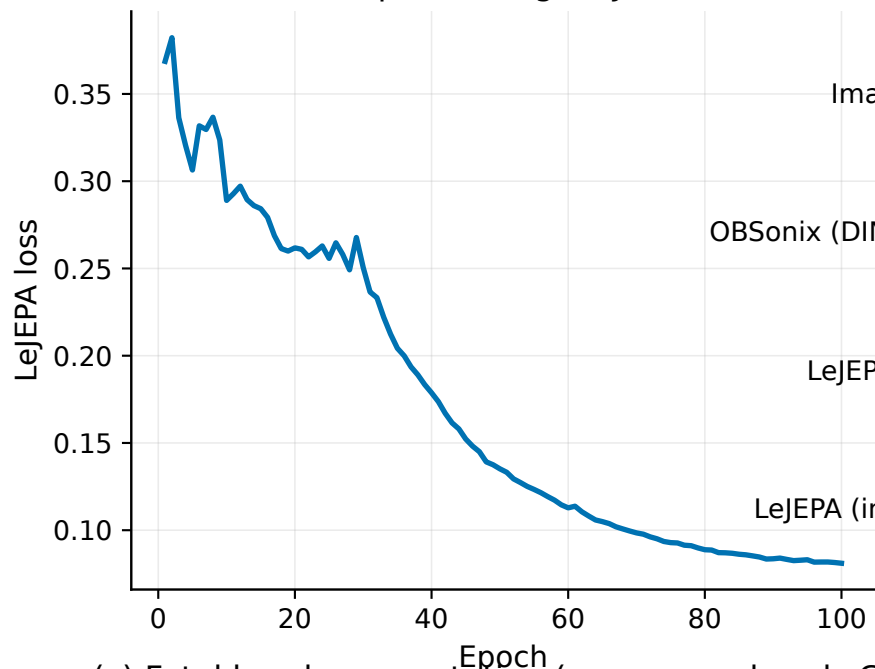

(b) Encoder initialization ablation

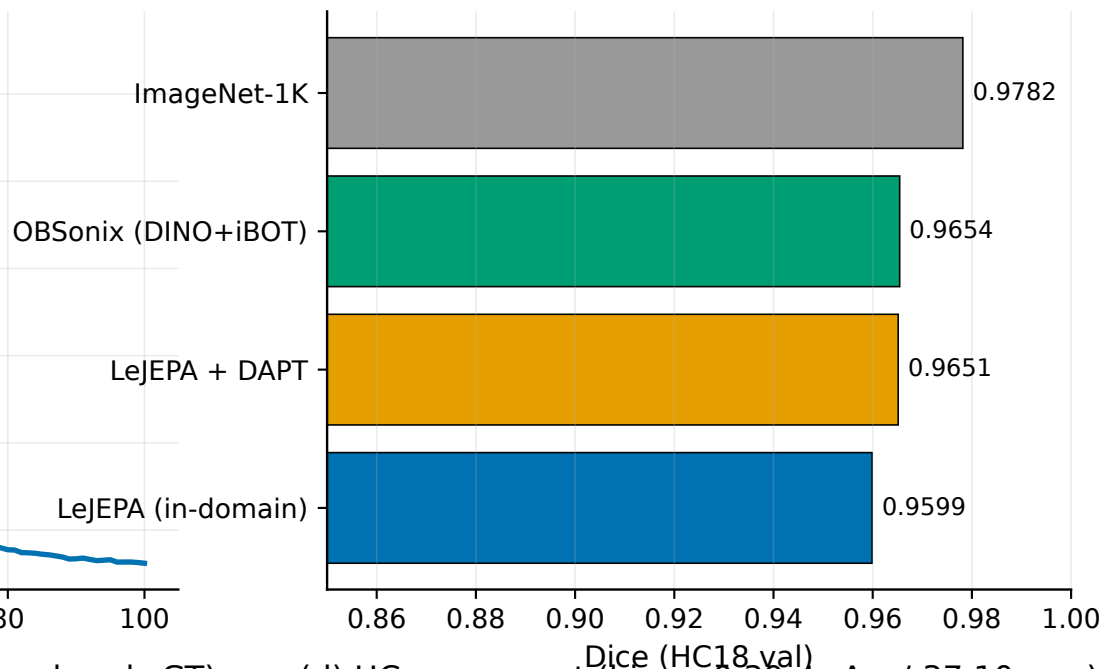

(c) Fetal head segmentation (green=pred, red=GT)

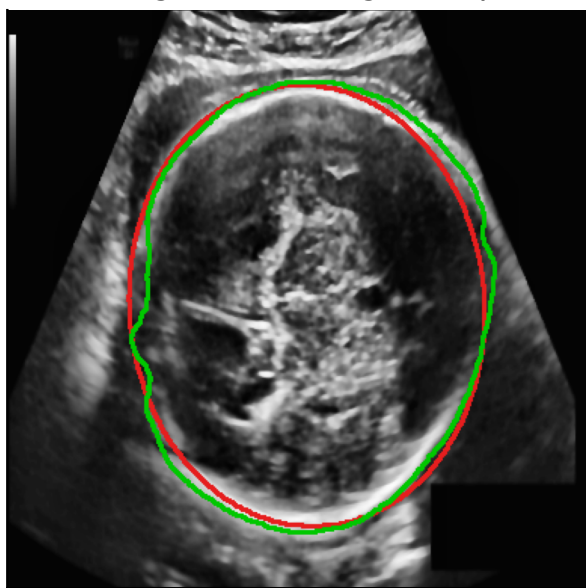

(d) HC agreement (bias=-0.39, LoA +/-37.10 mm)

