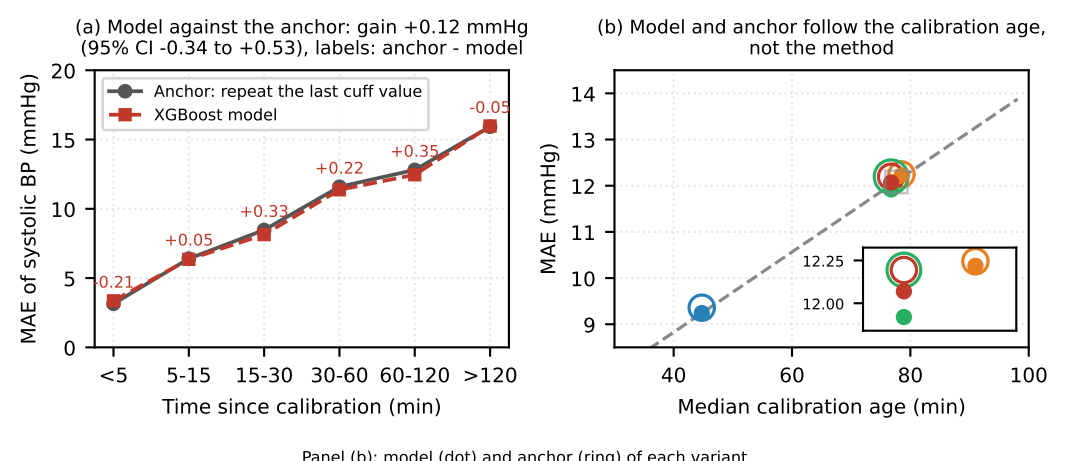
(a) Model against the anchor: gain +0.12 mmHg
(95% CI -0.34 to +0.53), labels: anchor - model
Anchor: repeat the last cuff value
XGBoost model
MAE of systolic BP (mmHg)
Time since calibration (min)
<5
5-15
15-30
30-60
60-120
>120
-0.21
+0.05
+0.33
+0.22
+0.35
-0.05
(b) Model and anchor follow the calibration age,
not the method
MAE (mmHg)
Median calibration age (min)
12.25
12.00
Panel (b): model (dot) and anchor (ring) of each variant
NeuroKit2: 28 subj., 17k windows, gain +0.12
Spectral (FFT): 40 subj., 49k windows, gain +0.03
Clinical covariates: 40 subj., 50k windows, gain +0.27
Baseline (own extraction): 40 subj., 50k windows, gain +0.12