

Can the eTemp Performance Sensor Reliably Measure Mean Skin Temperature During Exercise?

Felix Chen



Background & Aim

- Accurate skin temperature measurement during exercise is challenging due to sweating, movement and heat flux [1,2]
- Wearable sensors are increasingly used but require validation under dynamic physiological conditions

Aim: To assess agreement between the eTemp Performance sensor and a standard wired reference (Physitemp SST-1) for measuring mean skin temperature during rest, exercise and recovery.

Methods

- Simultaneous measurement using:
 - eTemp Performance sensor
 - Physitemp SST-1 (reference)
- Protocol: rest (15min) → exercise (30min) → recovery (15min)
- Participants: n = 14 (10 male, 4 female)
- Mean Skin Temperature: Ramanathan 4-site formula [3]



Key Results

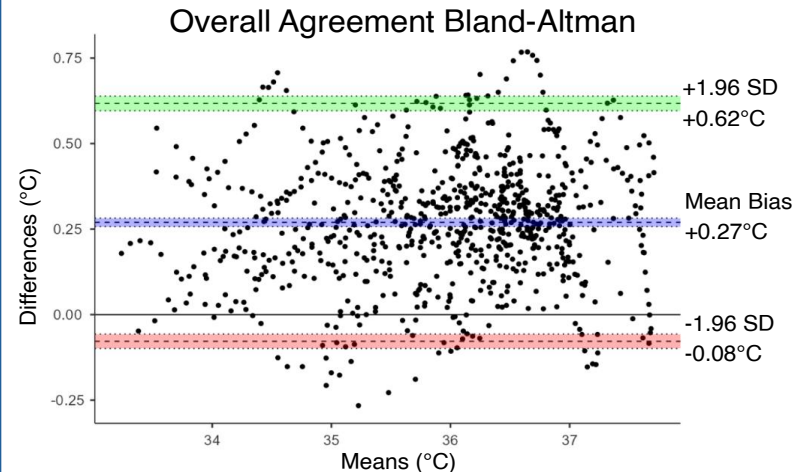


Figure 1- Agreement between the eTemp and Physitemp SST-1 sensors for mean skin temperature across the whole testing period (n=794) [4].

- **Mean bias:** +0.27°C
- **Limits of Agreement:** -0.08°C to 0.62°C
- **Mean absolute error:** 0.27°C
- Good overall agreement across all stages
 - Low mean bias and limits of agreement, within commonly accepted ranges

Exercise-specific findings

- Slightly higher bias and wider limits of agreement during exercise
- No meaningful proportional bias
- Measurement error remained small and independent of absolute temperature

Discussion

- eTemp slightly overestimated skin temperature versus Physitemp
- Bias was small and acceptable for exercise monitoring [4,5]
 - Agreement consistent across rest, exercise and recovery
- Differences likely due to sensor housing and surface area
- Physitemp has lower thermal mass may enhance evaporative cooling
- Overestimation represents a conservative error for heat strain monitoring

Future Perspectives

- Validation in outdoor exercise and occupational heat exposure
- Use in conservative safety thresholds where overestimation reduces risk
- Potential application in sport, military and clinical monitoring

References

1. Bach, A. J. E., Stewart, I. B., Minett, G. M., & Costello, J. T. (2015). Does the technique employed for skin temperature assessment alter outcomes? A systematic review.
2. Meade, R. D., Atkins, W. C., Bach, A. J. E., Foster, J., Hutchins, K. P., McKenna, Z. J., & Notley, S. R. (2024). Human heat resilience in a warming climate: Biophysical and physiological underpinnings of heat vulnerability and personal cooling strategies. *One Earth*, 7(8), 1343–1350. <https://doi.org/10.1016/j.oneear.2024.06.007>
3. Ramanathan, N. L. (1964). A new weighting system for mean surface temperature of the human body. *Journal of Applied Physiology*. (world). <https://doi.org/10.1152/jappl.1964.19.3.531>
4. Smith, A. D. H., Crabtree, D. R., Bilzon, J. L. J., & Walsh, N. P. (2010). The validity of wireless iButtons and thermistors for human skin temperature measurement. *Physiological Measurement*, 31(1), 95–114. <https://doi.org/10.1088/0967-3334/31/1/007>
5. Bandiera, D., de Bardonnèche, J., Janry, P., Calas-Étienne, S., Aubin, J.-C., Tessitore, A., Pitsiladis, Y., & Racinais, S. (2025). Validation of the iButton and Flex sensors for measuring skin temperature. *European Journal of Applied Physiology*. <https://doi.org/10.1007/s00421-025-06020-9>