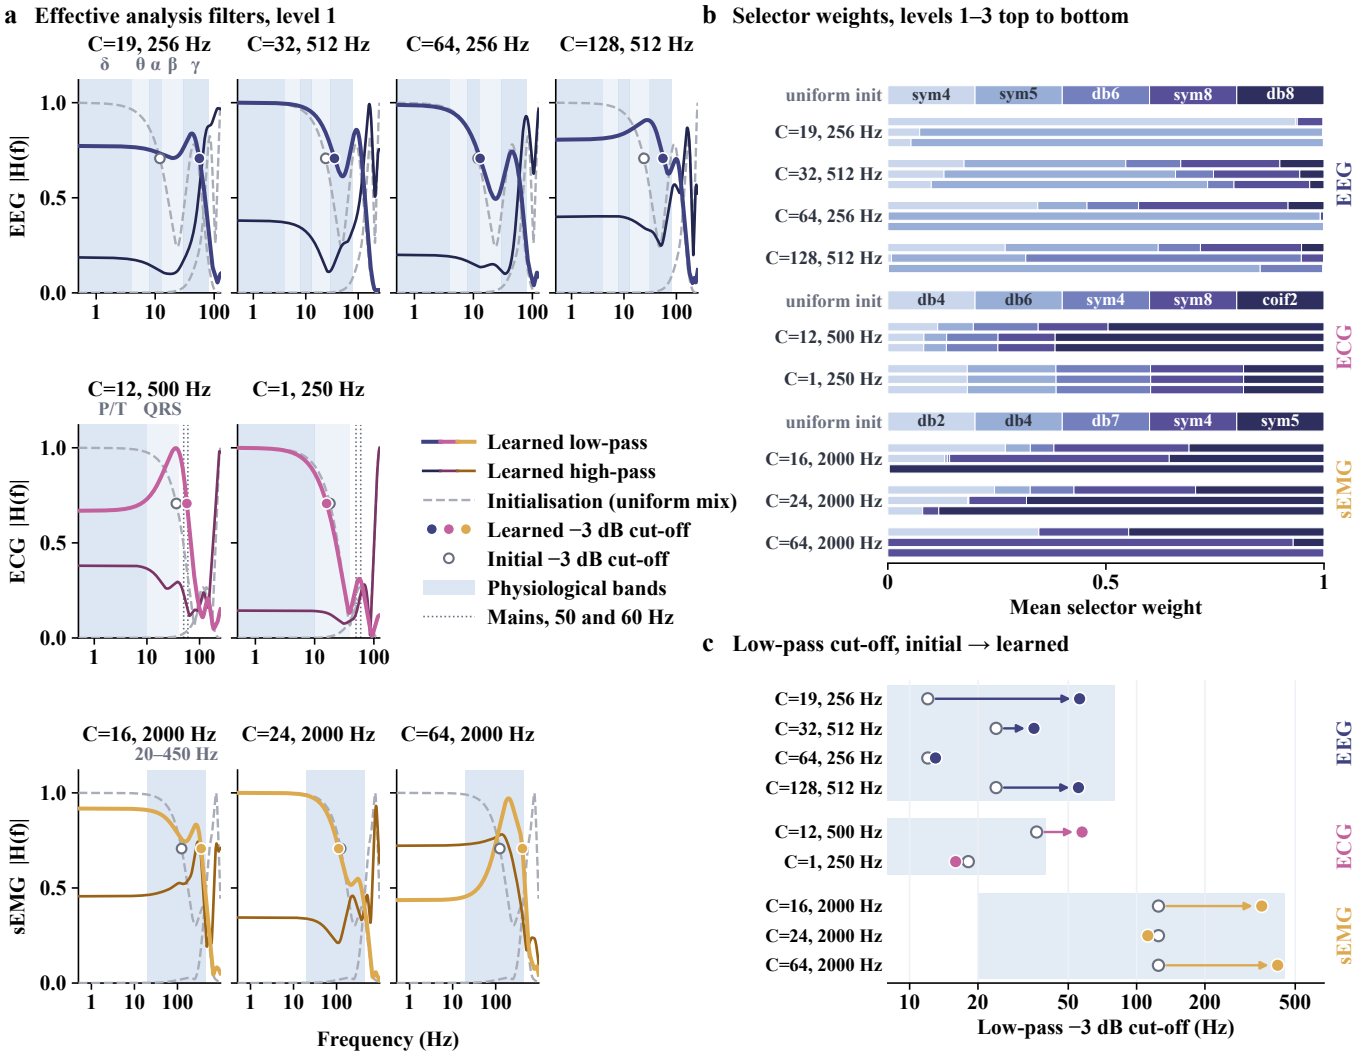

a Effective analysis filters, level 1
C=19, 256 Hz
C=32, 512 Hz
C=64, 256 Hz
C=128, 512 Hz
δ θ α β γ
EEG |H(f)|
C=12, 500 Hz
C=1, 250 Hz
P/T QRS
ECG |H(f)|
C=16, 2000 Hz
C=24, 2000 Hz
C=64, 2000 Hz
20–450 Hz
sEMG |H(f)|
Frequency (Hz)
Learned low-pass
Learned high-pass
Initialisation (uniform mix)
Learned −3 dB cut-off
Initial −3 dB cut-off
Physiological bands
Mains, 50 and 60 Hz
b Selector weights, levels 1–3 top to bottom
uniform init
sym4
sym5
db6
sym8
db8
C=19, 256 Hz
C=32, 512 Hz
C=64, 256 Hz
C=128, 512 Hz
EEG
uniform init
db4
db6
sym4
sym8
coif2
C=12, 500 Hz
C=1, 250 Hz
ECG
uniform init
db2
db4
db7
sym4
sym5
C=16, 2000 Hz
C=24, 2000 Hz
C=64, 2000 Hz
sEMG
Mean selector weight
c Low-pass cut-off, initial → learned
C=19, 256 Hz
C=32, 512 Hz
C=64, 256 Hz
C=128, 512 Hz
EEG
C=12, 500 Hz
C=1, 250 Hz
ECG
C=16, 2000 Hz
C=24, 2000 Hz
C=64, 2000 Hz
sEMG
Low-pass −3 dB cut-off (Hz)