sanas South African National Accreditation System

NON-CONFORMANCE, CORRECTIVE ACTION AND CLEARANCE REPORT

SANAS No.: T1195

Organisation Name: A Zurcsky PTY LTD

NC Report Number: NC03

Area/Scope Assessed: Coal testing

Assessor / Inspector / Expert: N Chilira

PART 1: DETAILED OBSERVATION

The Balance verification for Calorific Value Method does not cover the range as it only starts from 1g whereas 0,5g of the sample is weighed

Signed (Representative):

Signed (Team Leader / Inspector):

MAJOR: [X] MINOR: [ ]

Reference No. of relevant Guide / Standard / Requirement: ISO/IEC 17025 6.4

Date: 01/04/26

PART 2: ROOT CAUSE ANALYSIS

(Provide an analysis of the extent and cause of the nonconformity)

- Procedural misalignment between method requirements and equipment verification
- Inadequate technical review of the method.

PART 3: CORRECTIVE ACTION TAKEN

(Clearly indicate what corrective action was taken, and attach supporting evidence of implementation)

- Procurement of certified 500mg weight
- Balance ~~revision~~ verification template has been amended to include 0,5g(500mg) verification
- Communication to relevant personnel has been made for awareness of changes to the verification template.

Date: 04/05/2026

Signed (Representative): Mponya

PART 4: CORRECTIVE ACTION VERIFIED AND CLEARED

(Comment on whether the corrective action is sufficient and appropriate)

Date:

Signed: Assessor / Inspector/Expert:

PART 5: FOLLOW-UP AT NEXT ASSESSMENT

(Comment on the implementation of the corrective actions)

Date:

Signed: Assessor / Inspector/Expert:

©SANAS

AS004MF 07/25

BRAINSTORMING FORM

IRQ no: NC03

Brainstorming team

Keitumetse Maleka
Tshepo Mapanga
Sifiso Nyambi

What went wrong?

- The balance verification for calorific value method does not cover the range as it only starts from 1g wheas 0,5g of the sample is weighed.

Why? Why did the verification start at 1g?

- The material verification log was designed to only check from 1g

Why was the 0,5g weighing requirement overlooked?

- When the CV method was introduced into the scope, the balance verification was not cross-referenced against the methods standards minimum sample mass

Why was the lack of a 0,5g verification not caught interhally? When conducting audits, personel focused on whether verification was done, rather than the suitability of the range being verified

Reasons: Inadequate technical review

: Procedural misalignment between method requirements & verification of equipment.

Supervisor: Mapanga


AS001MF

07/25

ROOT CAUSE ANALYSIS FORM

IRQ NO: NC03

The balance verification for calorific value method does not cover the range as it only starts from 1g whereas 0.5g of the sample is weighed.

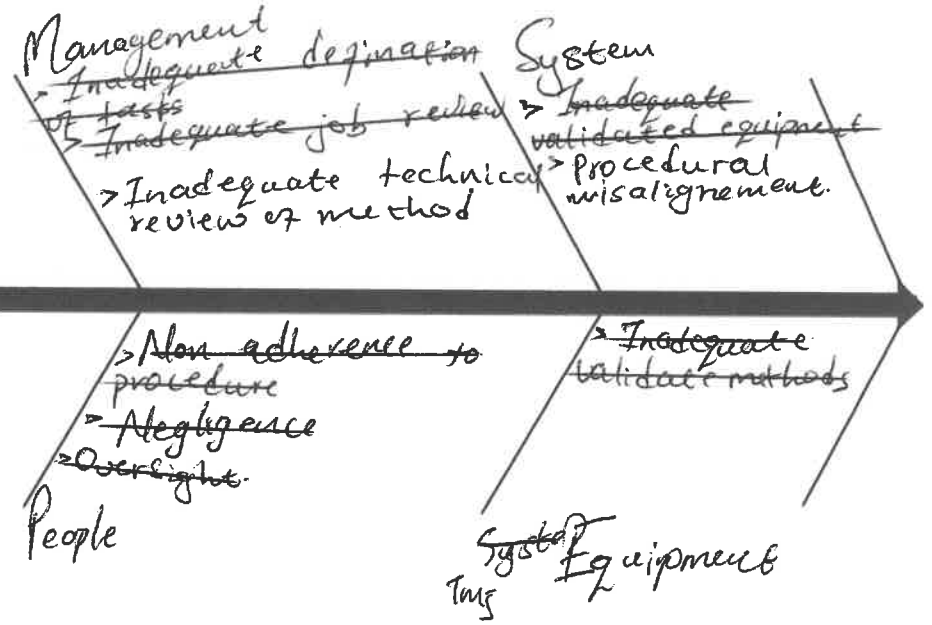

Aponya

SUPERVISOR

Tax Invoice

Date	24/04/2026
Page	1
Due By	31/05/2026
Document No	MEI28304

Micron Enterprises (Pty) Ltd
t/a Micron Equip (Pty) Ltd
Shop 5 & 7
Portion of Portion 234
292JS Farm Kromdraai
R565 Witbank 1035

Vat: 4140282619
Company Reg: 2018/066953/07
Tel: 013 690 1532
Fax: 013 656 1000

Azuresky (Pty) Ltd
37 5th Avenue
Lambton
Germiston
1401

Deliver to
Unit 3 ERF 534
17 Makriel Road
Wadeville
Germiston
1428

Account	Your Reference	Tax Exempt	Tax Reference	Sales Code		Incl/Excl
MEO03	EFT	N				Exclusive

Code	Description	Quantity	Unit	Unit Price	Disc%	Tax	Nett Price
ML-F1-500MG	Class F1 weight 500mg	1.00	EA	136.00		15.00%	136.00
ML-PCON-FR	Plastic Fraction Container	1.00	EA	85.00		15.00%	85.00
ML-CMASS	Calibration of Mass Pieces	1.00	EA	284.00		15.00%	284.00
ML-CERT	SANAS Calibration Certificate	1.00	EA	360.00		15.00%	360.00

Banking Details

ABSA BANK
Acc Nr: 409 391 8323
Branch Code: 632005
Saveways

PROCESSED BY: Mpumi

Received in good order

Date: 30-04-2026

Name: Nelson Sawis

Sign:

Sub Total		865.00
Discount @	0.00%	0.00
Amount Excl Tax		865.00
Tax		129.75
Total R		994.75

MICRON LABORATORY SERVICES

sanas Calibration Laboratory
CAL 103-03-00
CAL 103-14-00

9 Beatty Avenue, Witbank 1035 Tel: 013 690 1532 Fax: 013 656 1000
Postnet Suite 139 Private Bag X 7260 Witbank 1035
Reg No: 2017/365305/07 Vat nr: 4430102030
www.micronlab.co.za

CERTIFICATE OF CALIBRATION

Certificate no:	AZ WS1.1
Date of calibration:	21.04.2026
Date of next calibration:	30 April 2027
Customer:	AzureSky(Pty)Ltd. Unit 3 , 17 Makriel Road Wadeville Germiston
Location:	Laboratory
Contact:	nonhlanhla@azuresky.it.com

Conditions of Issue:

This certificate is issued in accordance with the conditions of accreditation granted by the South African National Accreditation System of South Africa. Subject to the uncertainties specified, this is a correct record of measurements made.

Copyright of this certificate is owned jointly by SANAS and the issuing laboratory. This certificate may not be reproduced other than in full without written approval of SANAS and of the issuing laboratory.

The values in this certificate were correct at the time of calibration. Subsequently the accuracy will depend on such factors as, the care of handling, the use of the instrument and the frequency of use. Re-calibrations should be performed after a period which has been chosen to ensure that the instrument's accuracy remains within the desired limits.

Where statements of conformity are made in the certificate, the following rules are applied:
Within Tolerance: Results ± expanded uncertainty within limits / specification.
Out of Tolerance: Results ± expanded uncertainty exceeds limits / specification.
Indeterminate: Results ± expanded uncertainty overlaps limits / specification.

Measurement results relate only to the item calibrated.

Technical Signatory: M Stroebel

Calibrated by: J Kruger

MICRON LABORATORY SERVICES

t +27 (0)13 690 1532 | f +27 (0)13 656 1000 | e admin@mlabs.co.za | 9 Beatty Avenue, Witbank, 1035
Postnet suite 139, Private bag X7260, Witbank, 1035

sanas Calibration Laboratory
CAL 103-03-00
CAL 103-14-00

CERTIFICATE OF CALIBRATION

Customer: AzureSky(Pty)Ltd.
Location: Laboratory
Date of Calibration: 21.04.2026
Date of Next Calibration: 30 April 2027

Certificate Number: AZ WS1.1
Weight Set: AZ WS1
Coy/Id Number: NN
Procedure Reference: P1.1.MP
Contact: nonhlanhla@azuresky.it.com

Weight ID	Nominal Value (g)	Actual Value (g)	Measurement Uncertainty (g) ±	Line Number
	0.5	0.500012	0.000012	1
ONE WEIGHT ONLY				

Procedure These weights have been calibrated on the basis of weighings made against standards of known mass and assumed density of **8000** kg/m³ traceable to the international standards.

Uncertainty The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor K=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Mass Density Should weighings be made requiring buoyancy correction, A density of 8000 kg/m3 should be assumed for these weights

Traceability **Standards Ref.No.** SET 1 **Re-Calibration Date:** 31 January 2028

Magnetism Weights were screened for magnetic influence prior to calibration no observable magnetic effects were detected.

Temperature 23.4 **°C ± 2°C** **Humidity** 44 **% ± 10%**

Remarks

Technical Signatory: M Stroebel

Calibrated By: J Kruger

End of Certificate

BEFORE

AzurESky		
AS019.3TF	BALANCE VERIFICATION	
Compiled by:	Sifiso Nyambi- Laboratory Manager	
Approved by:	Nonhlanhla Msibi- Operations Manager	

DAILY BALANCE VERIFICATION FORM

Equipment number:	AS2156									
Month:	1.0000 g	5.0000 g	10.0000g	20.0000g	50.0000g	100.0000 g	5.00 kg	Done by	Supervisor signature	Comments
Date	± 0.0002g	± 0.0003g	±0.0005g	± 0.0006g	±0.0005g	± 0.00010g	+0.05			
19/03/2026	0,9999	4,9999	10,0000	20,0001	50,0002	100,0001	-	RJ		
20/03/2026	0,9998	5,0000	10,0000	19,9999	50,0001	100,0000	-	LDP		
23/03/2026	1,0000	5,0001	9,9999	19,9999	50,0000	99,9999	-	NNH		
24/03/2026	1·0000	5·0002	9·9999	20·0002	50·0000	100·0000	-	LDP		
25/03/2026	1·0002	5·0000	10·0001	19·9998	50·0000	99·9998	-	NNH		
26/03/2026	1,0001	5,0003	10,0004	20,0005	50,0001	100,0006	-	K.M		
27/03/2026	1·0000	4·9999	10·0002	19,9997	50·0002	100·0002	-	AJ		
30/03/2026	1,0002	5,0000	10,0001	20,0003	50,0003	100,0004	-	N·N·H		
31/03/2026	0,9998	5,0003	10,0005	20,0004	50,0004	100,0003	-	K.M		
01/04/2026	1.0002	5·0002	10·0004	20·0003	50·0002	100·0004	-	A.J		

Document no	Revision Status	Effective Date	Next revision date
AS019.3TF	00	04/2025	04/2028

BEFORE

AzurESky		
AS019.3TF	BALANCE VERIFICATION	
Compiled by:	Sifiso Nyambi- Laboratory Manager	
Approved by:	Nonhlanhla Msibi- Operations Manager	

02/04/2026	1.0002	4.9999	10.0000	20.0004	50.0004	100.0007	-	NNH		
07/04/2026	1.0003	5.0003	10.0004	20.0002	50.0004	100.0004	-	AJ		
07/04/2026	1.0002	5.0003	10.0005	20.0003	50.0009	100.0005	-	SB		
08/04/2026	1.0001	5.0002	10.0004	20.0004	50.0006	100.0010	-	NNH		
09/04/2026	1.0001	5.0002	10.0001	20.0000	50.0004	100.0000	-	AJ		
13/04/2026	1.0002	5.0000	10.0003	20.0004	50.0004	100.0016	-	NNH		
14/04/2026	0.9999	4.9999	10.0003	20.0003	50.0006	100.0008	-	K.M		
15/04/2026	0.9998	5.0002	9.9998	20.0000	50.0000	100.0003	-	K.M		
16/04/26	1.0001	5.0002	10.0001	20.0003	50.0004	100.0008	-	K.M		
17/04/26	1.0001	5.0000	10.0000	20.0001	50.0004	100.0001	-	K.M		
20/04/26	0.9998	5.0001	10.0001	20.0004	50.0006	100.0009	-	NNH		
21/04/26	0.9998	4.9998	9.9999	20.0001	50.0001	100.0009	-	AJ		

ACTION

- **Tolerance limits exceeded 3 times successively**
- **Action limit exceeded**

Document no	Revision Status	Effective Date	Next revision date
AS019.3TF	00	04/2025	04/2028

AFTER

AzurESky	
AS019.2TF Rev 01	BALANCE VERIFICATION

Compiled by:	Sifiso Nyambi- Laboratory Manager	
Approved by:	Nonhlanhla Msibi- Operations Manager	

DAILY BALANCE VERIFICATION FORM

Equipment number:	AS00A31										
Month:	0.50000g	1.0000 g	5.0000 g	10.0000g	20.0000g	50.0000g	100.0000 g	5.00 kg	Done by	Supervisor signature	Comments
Date	± 0.0005g	± 0.0002g	± 0.0003g	±0.0005g	± 0.0006g	±0.0005g	± 0.00010g	+0.05			
04/05/2026	0,5001	1,0000	5,0002	10,0001	20,0001	49,9999	100,0001	~	KM		

Document no	Revision Status	Effective Date	Next revision date
AS019.2TF	01	04/2026	04/2028

AFTER

AzurESky		
AS019.2TF Rev 01	BALANCE VERIFICATION	
Compiled by:	Sifiso Nyambi- Laboratory Manager	
Approved by:	Nonhlanhla Msibi- Operations Manager	

ACTION

- **Tolerance limits exceeded 3 times successively**
- **Action limit exceeded**

Revision

Dated 04/05/2026, mass piece 0.5g was added to the verification set to account for range of analysis of methods involved within the scope.

AzurESky	**Document No.** AS008MF	**Page 1 of 1**
	Effective Date	**April 2026**
	Revision Date	**April 2029**
Title:	Memorandum	
Document by:	Azuresky Pty Ltd	**Revision No**
Compiled by:	Sifiso Nyambi & Tshepo Maponya	**00**
Authorizing Officer: N Msibi	**Signature:**	

Department: Analysis Room

Memorandum no: 009

Position: Laboratory Supervisor

Date: 07/05/2026

Title: Awareness of changes to template AS019TF

Kindly take note of the changes made on the balance verification template AS019TF, wherein there is now an addition of mass piece 0,5g. This has been done to cover the range of work for the laboratory's scope which starts from 0,5g in weighed masses. The template now aligns with the CABs range of analysis with this addition, as opposed to the previous template.

AzurESky	ATTENDANCE REGISTER		
	Document no:	Version:	Page:
	ASMF 17043-8.4.1	0	1
	Compiled by:	Sifiso Nyambi - Laboratory Manager	
	Approved by:	Nonhlanhla Msibi - Operations Manager	
Date:	04/05/2026		
Chair:	TMJ Maponya	Scribe	
Subject:	Awareness of changes to the verification of balance template A5019TF		
Absent:			

Present	Cell Number	Designation	Signature	Email address
NN Hlongwane	0723732558	Lab Analyst		nosipho@Azuresky.it.com
LD Photo	0766923263	Lab Analyst	Photo	lilo@azuresky.it.com
M. Maleka	071 724 9031	lab analyst	Maleka	keitumetse@azuresky.it.com
N. Mehlo	0827868449	Ops Manager		nonhlanhla@azuresky.it.com
A. Jama	0606111584	Lab analyst		abenathi@azuresky.it.com
TMJ Maponya	076 455 0692	Lab Supervisor		tshepo@azuresky.it.com