MICRON LABORATORY SERVICES

sanas Calibration Laboratory
CAL 103-03-00
CAL 103-14-00

9 Beatty Avenue, Witbank 1035 Tel: 013 690 1532 Fax: 013 656 1000
Postnet Suite 139 Private Bag X 7260 Witbank 1035
Reg No: 2017/365305/07 Vat nr: 4430102030
www.micronlab.co.za

SANAS Accredited Calibration Laboratory

CERTIFICATE OF CALIBRATION

Certificate no:	AZU VF1.2
Date of calibration:	27.02.2026
Date of next calibration:	March 2027
For:	AzureSky (Pty) Ltd Unit 3, 17 Markiel Road Wadeville Germiston, 1401
Location:	Laboratory
Contact:	nonhlanhla@azuresky.it.com

Conditions of Issue:

This certificate is issued in accordance with the conditions of accreditation granted by the South African National Accreditation System of South Africa. Subject to the uncertainties specified, this is a correct record of measurements made.

Copyright of this certificate is owned jointly by SANAS and the issuing laboratory. This certificate may not be reproduced other than in full without written approval of SANAS and of the issuing laboratory.

The values in this certificate were correct at the time of calibration. Subsequently the accuracy will depend on such factors as, the care of handling, the use of the instrument and the frequency of use. Re-calibrations should be performed after a period which has been chosen to ensure that the instrument's accuracy remains within the desired limits.

Where statements of conformity are made in the certificate, the following rules are applied:
Within Tolerance: Results ± expanded uncertainty within limits / specification.
Out of Tolerance: Results ± expanded uncertainty exceeds limits / specification.
Indeterminate: Results ± expanded uncertainty overlaps limits / specification.

Measurement results relate only to the item calibrated.

Technical Signatory: M Stroebel

Calibrated by: F Rossouw

MICRON LABORATORY SERVICES

t +27 (0)13 690 1532 | f +27 (0)13 656 1000 | e admin@mlabs.co.za | 9 Beatty Avenue, Witbank, 1035
Postnet suite 139, Private bag X7260, Witbank, 1035

sanas Calibration Laboratory
CAL 103-03-00
CAL 103-14-00

CERTIFICATE OF CALIBRATION


Customer:	AzureSky (Pty) Ltd	**Certificate Number:**	AZU VF1.2
Location:	Laboratory	**Instrument:**	ATS Volatile Furnace
Date of Calibration:	27.02.2026	**Serial Number:**	ATS/210325/59V
Date of Next Calibration:	March 2027	**Company Number:**	N.N
Contact:	nonhlanhla@azuresky.it.com	**Procedure Reference:**	P4.1.3.VOL ISO

Calibration Standards:	**Description**	**Model**	**Company No.**	**Re-calibration date**
	OMEGA LOGGER	HH309A (V 4.0.1.0)	V-DL26	30th November 2026

Temperature Recovery Rate Calibration Results - ºC

Time Interval	Before Calibration	After Calibration
Start	900	900
One Minute	780	780
Two Minute	844	844
Three Minute	882	882
Four Minute	895	895
Five Minute	898	898
Six Minute	900	900
Seven Minute	900	900
Overshoot	0	0
Uncertainty of Measurement	±	3

Recovery

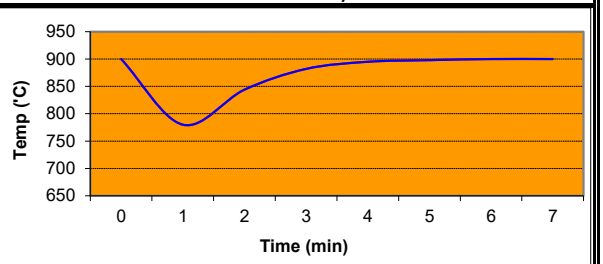


Method: The unit under test (UUT) was calibrated by comparison to the laboratory standard at the listed temperatures.

Temperture readings were taken over a period to include deviation from set point.

Unceratinty: The reported uncertainty of measurement stated as the standard uncertainty of measurement multiplied by the coverage factor K=2 which for a normal distribution corresponds to a coverage probability of approximatrly 95%.

The standard used for calibration are traceable to the national standard.

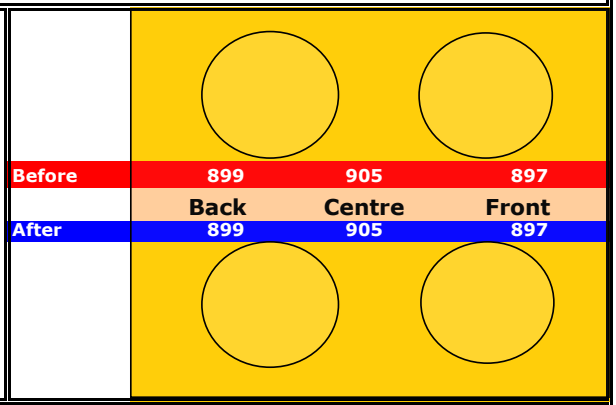

Controller Settings *(After Calibration Adjustment)*	Controller Off-Set °C	0	**Note: Adjustment to any of these** Controller settings will affect The unit accuracy, Ramp rate and Deviation from set point
	Proportional Band (P)	5	
	Ibtergration Time (I)	400	
	Derivate Time (D)	90	
Laboratory Enviroment During Calibration	**Temperature at start °C**	23	**± 2°C**
	Temperature at end °C	23	**± 2°C**
Remarks	**WITHIN TOLERANCE**		

Technical Signatory: M Stroebel

Calibrated By: F Rossouw


MICRON LABORATORY SERVICES

t +27 (0)13 690 1532 | f +27 (0)13 656 1000 | e admin@mlabs.co.za | 9 Beatty Avenue, Witbank, 1035
Postnet suite 139, Private bag X7260, Witbank, 1035

sanas Calibration Laboratory
CAL 103-03-00

CERTIFICATE OF CALIBRATION

Customer:	AzureSky (Pty) Ltd	**Certificate Number:**	AZU VF1.2
Location:	Laboratory	**Instrument:**	ATS Volatile Furnace
Date of Calibration:	27.02.2026	**Serial Number:**	ATS/210325/59V
Date of Next Calibration:	March 2027	**Company Number:**	N.N
Contact:	nonhlanhla@azuresky.it.com	**Procedure Reference:**	P4.1.3.VOL ISO

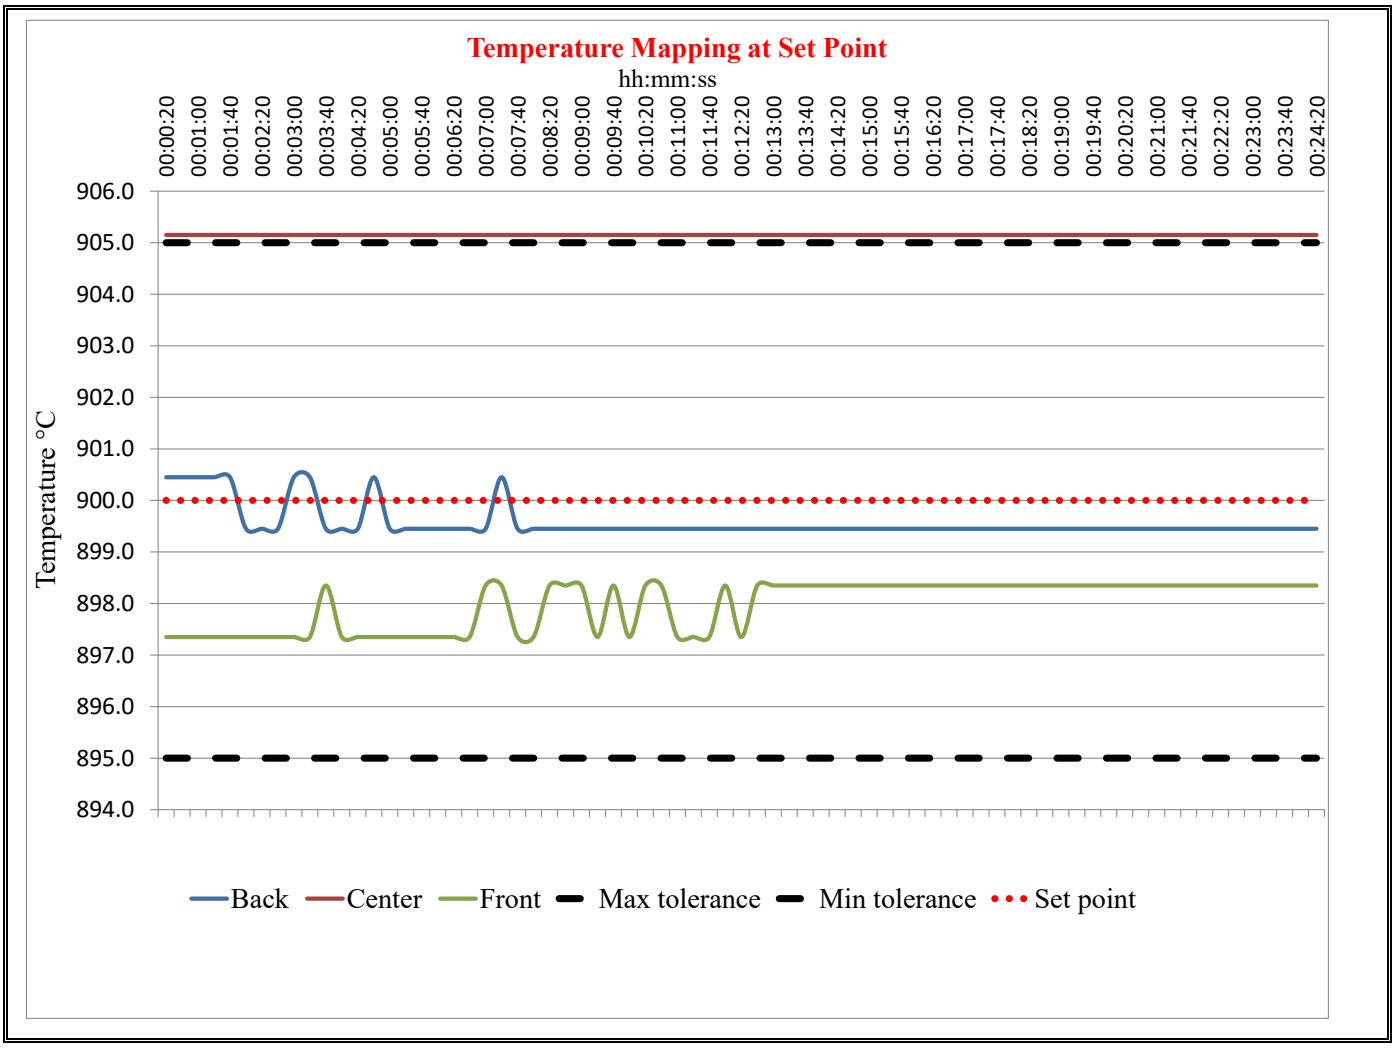

Technical Signatory: M Stroebel

Calibrated By: F Rossouw

End of Certificate