sanas South African National Accreditation System

NON-CONFORMANCE, CORRECTIVE ACTION AND CLEARANCE REPORT

SANAS No.:

Organisation Name: Mzuvestry Pty Ltd. | NC Report Number: NC10/2026 T

Area/Scope Assessed: Documentation | Assessor / Inspector / Expert: Tifiso M

PART 1: DETAILED OBSERVATION

The responsibility for authorising the resumption of work not clearly defined in 7.17. document.

Signed (Representative):

Signed (Team Leader / Inspector):

MAJOR: ☒ MINOR: ☐

Reference No. of relevant Guide / Standard / Requirement: ISO 17025 (SANAS F48-07 Cl 7.10).

Date: 02/09/2026

PART 2: ROOT CAUSE ANALYSIS

(Provide an analysis of the extent and cause of the nonconformity)

Due to incomplete System documentation, nowhere in the documented system clearly stated as to who gives authority for resumption of work.

PART 3: CORRECTIVE ACTION TAKEN

(Clearly indicate what corrective action was taken, and attach supporting evidence of implementation)

The drafting or updating the document (ASMF7.17) clearly stating that the operations / lab manager authorizes resumption of work

Date: 02/09/26

Signed (Representative):

PART 4: CORRECTIVE ACTION VERIFIED AND CLEARED

(Comment on whether the corrective action is sufficient and appropriate)

Addressed.

Date: 10/02/26

Signed: Assessor / Inspector/Expert:

PART 5: FOLLOW-UP AT NEXT ASSESSMENT

(Comment on the implementation of the corrective actions)

Date:

Signed: Assessor / Inspector/Expert:


©SANAS

AS001MF

07/25

ROOT CAUSE ANALYSIS FORM

IRQ NO: NC/10/2026 T

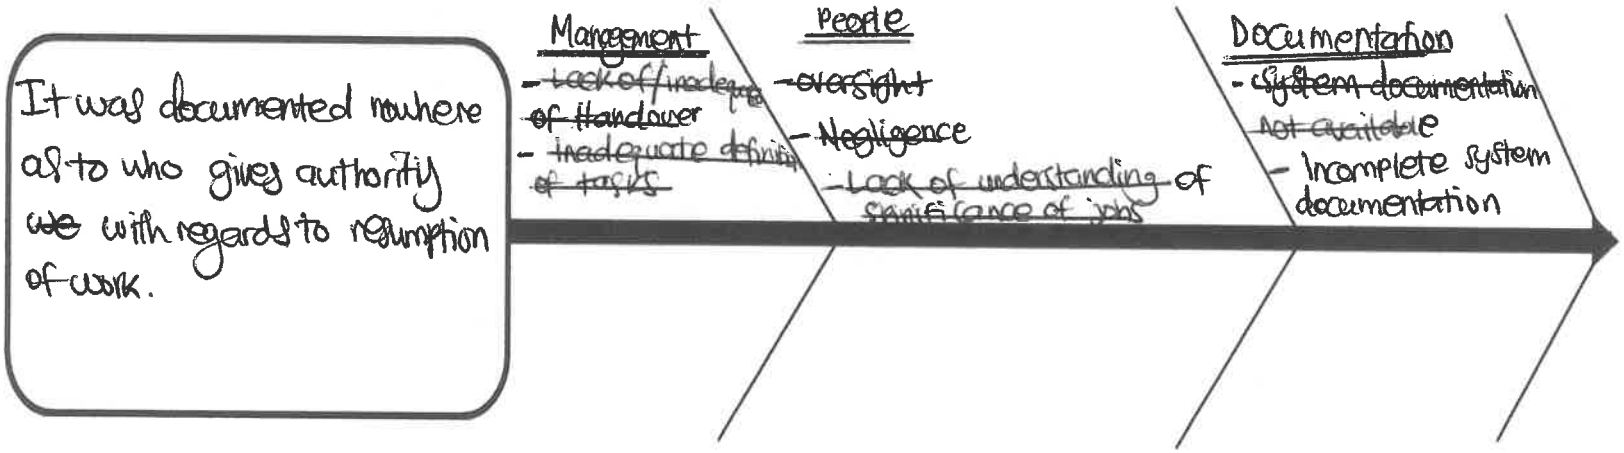

.....

SUPERVISOR

AS004MF 07/25

BRAINSTORMING FORM

IRQ no: NC10/2026T

Brainstorming team

Lilo Photo, Nosipho Hlongwane, Abenathi Jama, Tshepo Mapanya.

What went wrong? Nowhere was it stated in the documented as to who gives authority with regards to resumption of work.

Why 1 Why was it not clearly stated/documented in the system as to who authorizes resumption of work?

GAPS in the system, the laboratory was still being developed so there were no complete system documentation

Supervisor:

Before Before

AzurESky	MANAGEMENT OF NON-CONFORMING WORK (+17025)		
	Document no: ASMF7.17B		
	Compiled by:	Sifiso Nyambi - Laboratory Manager	
	Approved by:	Nonhlanhla Msibi - Operations Manager	

Laboratory Manager: Ensure compliance with ISO/IEC 17025 clauses 7.10 and 8.7 and ensure records are maintained

Lab Manager: Authorise suspension of testing where result validity is in question

Additional Procedure – ISO/IEC 17025 Nonconforming Work Handling

A. Identification of ISO/IEC 17025 Nonconforming Work

Nonconforming work may be identified from:

- QC failures or control chart breaches
- Failed method verification or validation checks
- Proficiency testing failures
- Equipment calibration out-of-tolerance results
- Deviations from approved test methods
- Review of test reports prior to release
- Complaints related to test/calibration results

B. Immediate Actions (ISO/IEC 17025 Context)

In addition to Section 5:

- Suspend testing or calibration activities where result validity may be compromised
- Quarantine affected test items or data
- Prevent release of affected reports
- Identify and segregate all work potentially affected

C. Evaluation of Impact on Results

The evaluation shall determine whether:

- Previously reported test/calibration results are invalid
- Customers require notification
- Results require withdrawal, amendment, or reissue
- Re-sampling or re-testing is required

CONTROLLED DOC

After

After

8. Corrective Actions

Once root cause is confirmed:

- Define the correction and corrective action
- Assign responsible personnel and target dates
- Validate effectiveness after implementation
- Document updates to SOPs, training, or process controls if needed
- Where necessary:
  - Ensure notification of customers and recall CRM's/RM's and certificates and documentation within an appropriate period. This also means that any tested samples which can have a significant impact on the operations of customers shall be relayed to the client.
  - PT reports already sent to participants are recalled or disregarded.

9. Follow-Up and Closure

- Verify the corrective action eliminated or mitigated the issue
- Retest or recharacterize RM/CRM/sample batch if necessary
- Document closure with review sign-off from operations/lab manager and resume work.
- Update NCW register and archive all records securely
- A planned Internal Audit must include the checking or evaluate the corrective action taken, this it ensures effectiveness of the implementation

CONTROLLED DOC