F 03-09

sanas South African National Accreditation System

NON-CONFORMANCE, CORRECTIVE ACTION AND CLEARANCE REPORT

SANAS No.:

Organisation Name: Zauresky Pty Ltd

NC Report Number: NC013/2026

Area/Scope Assessed: Document Review

Assessor / Inspector / Expert: Afise Nyamba

PART 1: DETAILED OBSERVATION

The Timelines to address NCs not specified.

Signed (Representative):

Signed (Team Leader / Inspector):

MAJOR: ☒ MINOR: ☐

Reference No. of relevant Guide / Standard / Requirement: ISO 17025 (Clause 8.7.1., SANAS F48-07)

Date: 06/02/2026

PART 2: ROOT CAUSE ANALYSIS

(Provide an analysis of the extent and cause of the nonconformity)

Incomplete System documentation

PART 3: CORRECTIVE ACTION TAKEN

(Clearly indicate what corrective action was taken, and attach supporting evidence of implementation)

Document ASMF7.17 was updated with correct/specified timeframes for closing/addressing non-conformances

Date: 06/02/26

Signed (Representative):

PART 4: CORRECTIVE ACTION VERIFIED AND CLEARED

(Comment on whether the corrective action is sufficient and appropriate)

Addressed

Date: 07/02/2026

Signed: Assessor / Inspector/Expert:

PART 5: FOLLOW-UP AT NEXT ASSESSMENT

(Comment on the implementation of the corrective actions)

Date:

Signed: Assessor / Inspector/Expert:


©SANAS

AS001MF

07/25

ROOT CAUSE ANALYSIS FORM

IRQ NO: NC3-2026 T

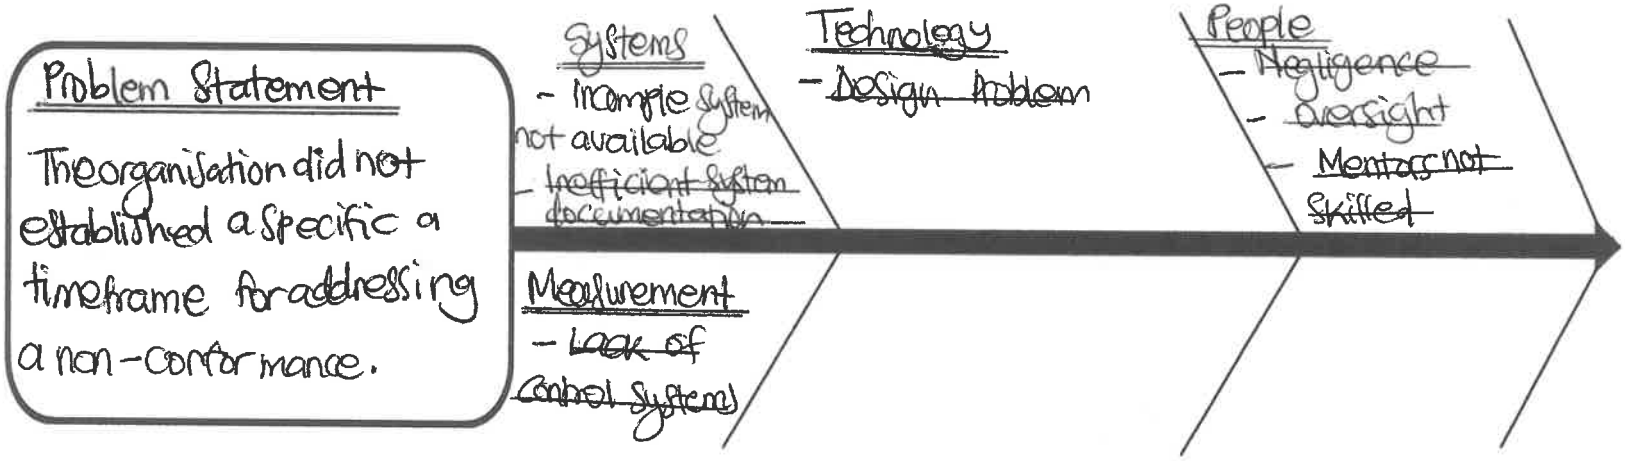

.....

SUPERVISOR

AS004MF 07/25

BRAINSTORMING FORM

IRQ no: NC13-2026T

Brainstorming team

Lilo Dorothy Photo, Nosiphotlhongwane, Tsheps Maponya, Abenathi Jama and Keitumetse Maleka.

Problem Statement: The organisation did not establish a specified timeframe for addressing a non-conformances.

Why 1? Why is there no defined timeframe for resolving non-conformances within the current processes?

There is a Non-Conformances procedure, however it did not address the timeframes for non-conformances.

Supervisor: Maponya

Before

	MANAGEMENT OF NON-CONFORMING WORK	
AzurESky	Document no: ASMF7.17	
Compiled by:	Sifiso Nyambi - Laboratory Manager	
Approved by:	Nonhlanhla Msibi - Operations Manager	

Role	Responsibility
Lab analyst/ operator	Report and document non-conforming work immediately
Operations Manager	Approve final corrective actions and ensure traceability of decisions

4. Identification of non-conformity

Sources may include:

- Observation during routine work or supervision
- Internal audits
- Stability/homogeneity test failures
- Customer complaints
- Out-of-spec test results
- Incorrect CoA's or labelling errors

5. Initial Actions

- Immediately halt use of affected PT or RM/CRM or analysis or process step.
- Label the product or isolate the equipment with "NON-CONFORMING" tags.
- Notify the Laboratory/Operations Manager.
- Use ASMF 8.7.3 Improvement Action request form

CONTROLLED DOC

Effective date	Rev status	Next review date
02/2026	02	02/2029

Before

6. Documentation

The Improvement Action request form shall log the following:

- Unique NCW ID
- Date/time of detection
- Process stage affected
- Description of non-conformance
- Responsible person(s)
- Immediate action taken (containment),If necessary, ensure notification to customers within 24 hours of recording an NCW
- Signature of person reporting

7. Evaluation and Risk Assessment

Assess whether the non-conformance:

- Affects previously released PT or RMs/CRMs
- Affects previously released reports/work/samples tested.
- Requires rework, retesting, or full recall
- Risks invalidating assigned property values or traceability
- Has occurred before (recurring issue)

Use a **risk matrix** to evaluate severity and urgency.

CONTROLLED DOC

Before

8. Corrective Actions

Once root cause is confirmed:

- Define the correction and corrective action
- Assign responsible personnel and target dates
- Validate effectiveness after implementation
- Document updates to SOPs, training, or process controls if needed
- Where necessary:
  - Ensure notification of customers and recall CRM's/RM's and certificates and documentation within an appropriate period. This also means that any tested samples which can have a significant impact on the operations of customers shall be relayed to the client.
  - PT reports already sent to participants are recalled or disregarded.

9. Follow-Up and Closure

- Verify the corrective action eliminated or mitigated the issue
- Retest or recharacterize RM/CRM/sample batch if necessary
- Document closure with review sign-off from operations/lab manager and resume work.
- Update NCW register and archive all records securely
- A planned Internal Audit must include the checking or evaluate the corrective action taken, this it ensures effectiveness of the implementation

CONTROLLED DOC

After

4. Identification of non-conformity

Sources may include:
- Observation during routine work or supervision
- Internal audits
- Stability/homogeneity test failures
- Customer complaints
- Out-of-spec test results
- Incorrect CoA's or labelling errors

5. Initial Actions

- Immediately halt use of affected PT or RM/CRM or analysis or process step.
- Label the product or isolate the equipment with "NON-CONFORMING" tags.
- Notify the Laboratory/Operations Manager.
- Use ASMF 8.7.3 or SANAS F03-09 Improvement Action request form.

6. Documentation

The Improvement Action request form shall log the following:
- Unique NCW ID
- Date/time of detection
- Process stage affected
- Description of non-conformance
- Responsible person(s)
- Immediate action taken (containment), If necessary, ensure notification to customers within 24 hours of recording an NCW
- Signature of person reporting

ADDED:
- Root cause(s) identified
- Corrective action(s) taken
- Evidence of implementation

After

- Planned date for effectiveness review
- Results of effectiveness review
- Date of closure

7. Evaluation and Risk Assessment

Assess whether the non-conformance:
- Affects previously released PT or RMs/CRMs
- Affects previously released reports/work/samples tested
- Requires rework, retesting, or full recall
- Risks invalidating assigned property values or traceability
- Has occurred before (recurring issue)

Use a risk matrix to evaluate severity and urgency.

8. Corrective Actions

Once root cause is confirmed:
- Define the correction and corrective action
- Assign responsible personnel and target dates
- Validate effectiveness after implementation
- Document updates to SOPs, training, or process controls if needed

ADDED:
- Where necessary, changes to the management system (procedures, work instructions, risk registers, or controls) shall be implemented to prevent recurrence of the non-conformance.
- Appropriate corrective actions shall be proportional to the risk and impact of the non-conforming work.
- All corrective actions shall be traceable to the identified root cause.

- Where necessary:

After

- Ensure notification of customers and recall CRM's/RM's and certificates and documentation within an appropriate period. This also means that any tested samples which can have a significant impact on the operations of customers shall be relayed to the client.
- PT reports already sent to participants are recalled or disregarded.

9. Follow-Up and Closure

• Verify the corrective action eliminated or mitigated the issue
• Retest or recharacterize RM/CRM/sample batch if necessary
• Document closure with review sign-off from operations/lab manager and resume work.
• Update NCW register and archive all records securely
• A planned Internal Audit must include the checking or evaluate the corrective action taken, this it ensures effectiveness of the implementation

ADDED:
• Effectiveness of corrective actions shall be evaluated after a suitable period of implementation to confirm that the non-conformance has not recurred and that process performance has improved.
• Effectiveness shall be verified by review of subsequent test results, repeat stability or homogeneity testing (where applicable), audit findings, or trend analysis of NCW records.
• The outcome of the effectiveness review shall be recorded on the Improvement Action Request form prior to formal closure of the NCW.

10. Timelines

• Major NCs shall be closed within 24 hours from the time of detection.
• Minor NCs shall be closed within 7 days from the time of detection.

ADDED:
• Effectiveness of corrective actions for **Major NCs** shall be reviewed within **1 to 3 months**, depending on the nature and risk of the non-conformance.