sanas South African National Accreditation System

NON-CONFORMANCE, CORRECTIVE ACTION AND CLEARANCE REPORT

SANAS No.:

Organisation Name: Azuresky PTY LTD

NC Report Number: NC16-2026

Area/Scope Assessed: System documentation

Assessor / Inspector / Expert: Mapoya Tshepo

PART 1: DETAILED OBSERVATION

During the review, it was noted that not all performance characteristics were evaluated in the report, AS003MU and no valid reason provided.

Signed (Representative):

Signed (Team Leader / Inspector):

MAJOR: ☑ MINOR: ☐

Reference No. of relevant Guide / Standard / Requirement: 7.2.2

Date: 06/02/2026

PART 2: ROOT CAUSE ANALYSIS

(Provide an analysis of the extent and cause of the nonconformity)

The original validation report focused on the parameters making the method sufficiently Fit for purpose, but omitted to include the reason for the ommission, thereby making the non-conformance classified as incomplete system documentation.

PART 3: CORRECTIVE ACTION TAKEN

(Clearly indicate what corrective action was taken, and attach supporting evidence of implementation)

A section within method validation AS003MU has been included to outline reasons to justify why other performance characteristics are not covered.

Date: 06/02/26

Signed (Representative):

PART 4: CORRECTIVE ACTION VERIFIED AND CLEARED

(Comment on whether the corrective action is sufficient and appropriate)

Addressed

Date: 06/02/25

Signed: Assessor / Inspector/Expert:

PART 5: FOLLOW-UP AT NEXT ASSESSMENT

(Comment on the implementation of the corrective actions)

Date:

Signed: Assessor / Inspector/Expert:

©SANAS

BRAINSTORMING FORM

IRQ no: NC:16/2026

Brainstorming team

Nosipho N Hlongwane, Abenathi Jama, Keitumetse Maleka & Sifiso Nyambi

Problem Statement: Not all performance characteristics were evaluated in the AS003MV report and no valid reason provided.

Why one: Why was no Justification provided for the excluded performance characteristics?

The original validation report focused on the parameters or performance characteristics that make the method sufficiently fit for purpose. ~~Therefore~~


Supervisor:

AS001MF

07/25

ROOT CAUSE ANALYSIS FORM

IRQ NO: NC16/8026

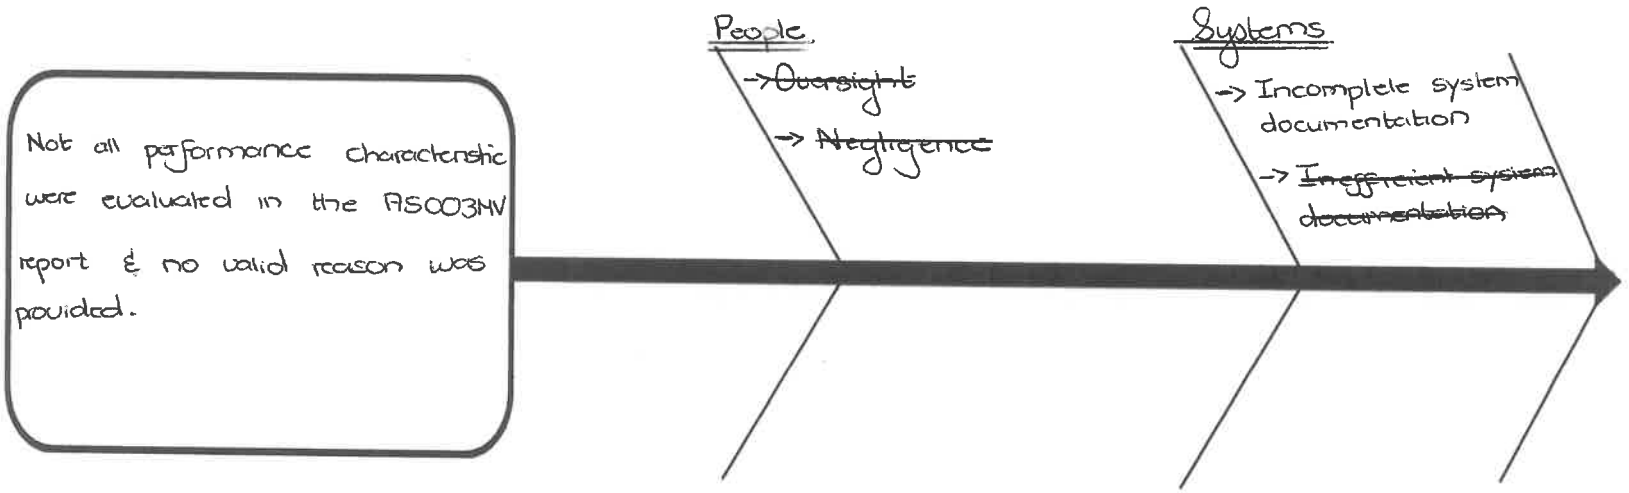

.....

SUPERVISOR

Before

AzurESky "ensure quality of test"	AzureSky		
	Method Validation for Ash Determination		Document no: AS003MV
	Compiled by:	Tshepo Maponya – Laboratory Supervisor	
	Approved by:	Nonhlanhla Msibi -Operations Manager	

CONTROLLED DOCUMENT

Performance Characteristics

Performance characteristics are the key parameters to be addressed to ensure the method is fit for its intended purpose.

Accuracy

Accuracy - The accuracy of an analytical method is the extent to which test results generated by the method and the true value agree. Accuracy can also be described as the closeness of agreement between the value that is adopted, either as a conventional, true, or accepted reference value, and the value found.

A sample of known value CRM AS002 was analysed 10 times, with the results captured as follows:

LIMS NO	Original	Duplicate	Average
1337	22.08	22.17	22.13

Effective date	Rev status	Next review date
07/2025	00	07/2028

1338	22.10	21.92	22.01
1339	22.59	22.54	22.57
1340	22.55	22.69	22.62
1341	22.60	22.47	22.53
1342	22.36	22.74	22.55
1343	22.67	22.5	22.58
1344	22.61	22.72	22.67
1345	22.64	22.61	22.62
Overall average			**22.48**
Standard deviation			**0.23559**

Percentage recovery

$$\%\text{Percentage Recovery} = \left(\frac{\text{ReferenceValue}}{\text{Validation Average}}\right) * 100$$

$$= \left(\frac{22.50}{22.48}\right) * 100$$

$$= 100.089\%$$

- 100.089% is extremely close to 100%, indicating very high agreement with the reference value.

CONTROLLED DOCUMENT

AzurESky "ensure quality of test"	AzureSky	
	Method Validation for Ash Determination	Document no: AS003MV
	Compiled by:	Tshepo Maponya – Laboratory Supervisor
	Approved by:	Nonhlanhla Msibi -Operations Manager

Characteristic (per TR 26)	Technical Justification for Omission
Limit of Detection (LOD)	Ash determination is a macro-analytical gravimetric method used to quantify bulk components, not trace levels. The LOD is not a critical parameter because the ash content in the samples (Hardcoal) is significantly higher (typically >1%) than the detection limits of the analytical balance (0.0001g).
Limit of Quantitation (LOQ)	Similar to LOD, the LOQ is not applicable for high-mass gravimetric analysis. The method is designed to measure total inorganic residue where the result is far above the "noise" level of the measurement system.
Linearity	Linearity is applicable to instrumental methods using calibration curves (e.g., ICP or UV-Vis sulphur analyzers). For gravimetric Ash determination, the relationship between the analyte (mass) and the result is inherently linear based on the laws of physics. No calibration curve is generated; therefore, linearity studies are not technically relevant.
Selectivity / Specificity	Selectivity in Ash determination is operationally defined by the method conditions (e.g., incineration at 815°C ± 10°C for coal). The method is non-specific by design, as it measures the total residue remaining after oxidation. Potential interferences are addressed via the temperature control and atmosphere specified in the ISO standard.

Effective date	Rev status	Next review date
02/2026	01	02/2029

CONTROLLED DOCUMENT

	AzureSky		
AzurESky "ensure quality of test"	**Method Validation for Ash Determination**	**Document no: AS003MV**	
	Compiled by:	**Tshepo Maponya – Laboratory Supervisor**	
	Approved by:	**Nonhlanhla Msibi -Operations Manager**	

Characteristic (per TR 26)	Technical Justification for Omission
Stability	The analyte (Ash/Inorganic residue) is the stable remains of a combustion process. Once the sample has been cooled in a desiccator to a stable mass, the residue is chemically inert and stable. Stability of the final residue is managed by the "cooling to constant mass" protocol within the procedure itself.

Revision

Revision no	Content changed	Reason for revision
01	No changes, additional information inserted which is a table for justification of omission of performance characteristics	Incomplete documentation, improvement to suffice TR-26

Effective date	Rev status	Next review date
02/2026	01	02/2029

CONTROLLED DOCUMENT